Apteryx Inc.
313 S. High St. Suite 200
Akron, OH 44308

330-376-0889 voice
330-376-0788 fax
sales@apteryx.com
www.apteryx.com

XVLite™
User Manual

Abstract

This document contains work instructions related to utilizing the dental imaging application, XVLite™ version 3.12 and above.

Copyright © 2004-2011 Apteryx, Inc. Apteryx® is a registered trademark of Apteryx, Inc.
All rights reserved. All other trademarks and tradenames are the property of their respective owners.

Controlled Document: *Printed or downloaded copies are considered uncontrolled and are for reference only.*

REVISION HISTORY

Revision Level	Revision Date	Description of Revision	Effective Date	Revision Author (Initials)	Approver(s) (Initials)	Doc Change Task#
DRAFT	6/10/2010	Draft	NA	SN		
1.0	8/22/2011	Initial Release	8/22/2011	SN	PW	
2.0	10/10/2011	Updated document formatting to comply with new doc control conventions	10/17/2011	SN	PW	85
2.1	02/21/2012	• Repl. Adv imaging Enh.Alg. with Real-Time Filters (new feature in 3.12.0.15). • Changed path to access Doc Templates.	05/24/2012	SN/BT	PW	128

TABLE OF CONTENTS

Revision History 2
Table of contents 3
1 THE USER INTERFACE 5
1.1 General Overview 5
2 MANAGING PATIENTS 6
2.1 Open/Create Patients Using a Practice Management Bridge 6
2.2 Adding/Creating a New Patient 6
2.3 Editing Patient Information 7
2.4 Deleting a Patient 7
2.5 Viewing an Existing Patient's Images 8
2.6 Viewing a Group/Series of Images 11
3 CAPTURING IMAGES FROM A X-RAY SENSOR/UNIT 12
3.1 Capturing Single Images from a X-ray Sensor/Unit 12
3.2 Capturing a Group/Layout Images from an X-ray Sensor/Unit 15
4 CAPTURING IMAGES FROM SCANNERS 18
4.1 General Information 18
4.2 Capturing Single Images from a Scanner 18
4.3 Capturing Group/Layout Images from Scanner 20
5 CAPTURING IMAGES FROM AN INTRA-ORAL CAMERA 24
5.1 General Information 24
5.2 Capturing Single Images from an IO Camera 24
5.3 Capturing Group/Layout Images from an IO Camera 27
6 IMAGE ENHANCEMENT 30
6.1 General Information 30
6.2 Accessing Image Enhancement Options 30
6.3 Brightness/Contrast 31
6.4 Sharpening 33
6.5 Noise Removal 34
6.6 Real-Time Filters 35
7 LABELLING IMAGES 38
7.1 General Information 38
7.2 Adding and Modifying Labels, Markers and Annotations 38
7.3 Calibrating Images and Adding Measurement Labels 40
8 DISTRIBUTING IMAGES – TRANSIT™ ADD-ON COMPONENTS 45
8.1 General Information 45
8.2 TransIT™ General Emailer Creator 45
8.3 TransIT™ Emailer Creator 48
8.4 FastAttach by NEA 50
8.5 XrayView™ e-Mailer Creator 55
8.6 XrayView™ Creator 60
9 PRINTING IMAGES AND IMAGE-RELATED DOCUMENTS 65
9.1 General Information 65
9.2 Printing a Single Image 65
9.3 Printing Multiple Images 65
9.4 Printing Images in a Layout/Group/Series 67
9.5 Document Templates 69
10 APPENDIX A: COMMON FUNCTIONS AND UTILITIES 74
10.1 Importing Images from an External Source 74
10.2 Deleting a Patient's Images 76
10.3 Finding Images by Date 77
11 APPENDIX B: CUSTOMIZING LAYOUT DEFINITIONS 80
11.1 General Information 80
11.2 Overview of the 'Layout Definition' Dialog Box 80

11.3 Common Layout Tasks: Changing the Capture Order 82
11.4 Common Layout Tasks: Changing the Capture Source 82
11.5 Common Layout Tasks: Adding Tiles 83
11.6 Common Layout Tasks: Creating New Layouts Based on Existing Layouts 83
12 APPENDIX C: CONFIGURING DOCUMENT HANDLING OPTIONS 85
12.1 Overview 85
12.2 Configuring Document Template Options 85
13 APPENDIX D: CONFIGURING PREFERENCES 87
13.1 General Information 87
13.2 General Preferences 87
13.3 Interface Preferences 88
13.4 Sensor Preferences 90
13.5 Imaging Options and Preferences 91
13.6 Print Preferences 92
13.7 Database Preferences 93
13.8 Advanced Preferences 94

1 THE USER INTERFACE

1.1 General Overview

The imaging application provides a wizard-driven interface designed to make the image capturing and viewing process intuitive and simple.

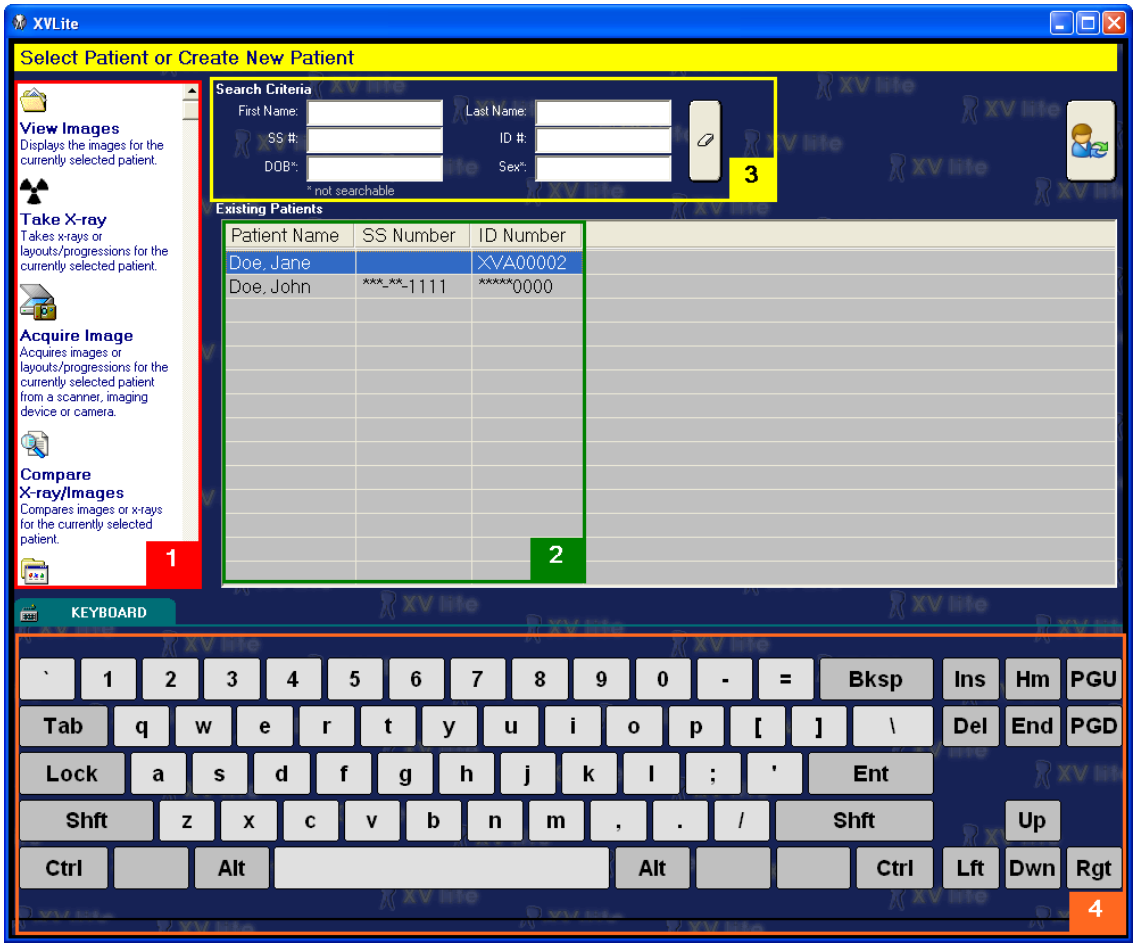

- **1- Main Menu Bar:** The main navigation menu. Provides wizard-driven access to functions such as: viewing images; taking X-rays from sensors; or acquiring images from devices such as flatbed: scanners; intra-oral camera; and panoramic/cephalometric systems.
- **2 - Existing Patients List:** Displays the current list of patients that exist in the patient database.
- **3 - Patient Search Entry Form:** Allows users to search the patient database.
- **4 - Touch screen Keyboard (Optional):** If selected, a keyboard displays for touch screen monitors typically used in dental operatories.

2 MANAGING PATIENTS

2.1 Open/Create Patients Using a Practice Management Bridge

The imaging application provides users numerous methods to create or open patient records. Although patient records can be manually created, the most common method employed by dental practices is through integration referred to as a Practice Management (PM) Bridge.

PM Bridging automates the patient creation process by "carrying over" patient (first name, last name, id number, SS number) and demographic (birth date, gender, etc.) information from common, third-party PM application to the imaging application. PM bridging assures that patient information in the imaging application matches the information contained in the PM application.

A PM bridge can be established using the following methods:

- NameGrabber™ - Apteryx's patented applet. When installed, NameGrabber runs in the Windows System Tray. Users simply open a patient's record in the PM application by and then click on the NameGrabber icon in the system tray. The imaging application is automatically launched, the patient's information is carried over, and the patient's record is opened or created. Visit www.apteryx.com for more information.
- PM DataDrills – Thru the use of Apteryx's PM data drills, the imaging application can manually "pull" patient and related demographic information directly from a third-party PM database and use it to create a patient. DataDrills are typically used in conjunction with NameGrabber to fill in any missing information when pulling patient data from an application. Visit www.apteryx.com for more information.
- Integrated PM Bridge / Command Line Options – The imaging application offers many options to open patients using command line arguments. Parameters can be "sent" with the application's executable file to open/create patients. Command line options are useful to developers for creating a button within a third-party PM application that automates the process of opening or creating the related patients image file. For more information refer to the following online knowledgebase article: OVERVIEW: Command Line Parameters.

In many circumstances, before a PM bridge is implemented, a dental practice manually creates patients in the software. As a result, patient information may not exactly match the information being passed via the PM bridge. After the PM bridge is implemented, the user may be presented with a 'Patient Does Not Exist' dialog box when attempting to open a patient that DOES exist in the imaging application if there is a mismatch with the patient information passed. Refer to the following online knowledgebase article for instructions to update the existing patient: HELP: Error "Patient Does Not Exist".

2.2 Adding/Creating a New Patient

To manually create a new patient record:

2.2.1 Enter in the required patient information in the 'Search Criteria' fields. The following restrictions are placed on the following entries:

- 'SS Number'
  - Maximum of 16 characters
  - Can contain characters, digits or symbols
- 'ID Number'
  - Maximum of 64 characters
  - Can contain characters, digits or symbols

2.2.2 Scroll down on the main navigation if necessary and select **Create Patient**.



2.2.3 The 'Existing Patients' list will refresh to display the new patient record.

2.3 Editing Patient Information

To modify an existing patient's record:

2.3.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

2.3.2 Select the patient's record and then select **Advanced Patient Options > Edit Patient Information** on the menu bar.

2.3.3 Add/Modify any of the provided fields as desired and then click on **OK** to save the changes.

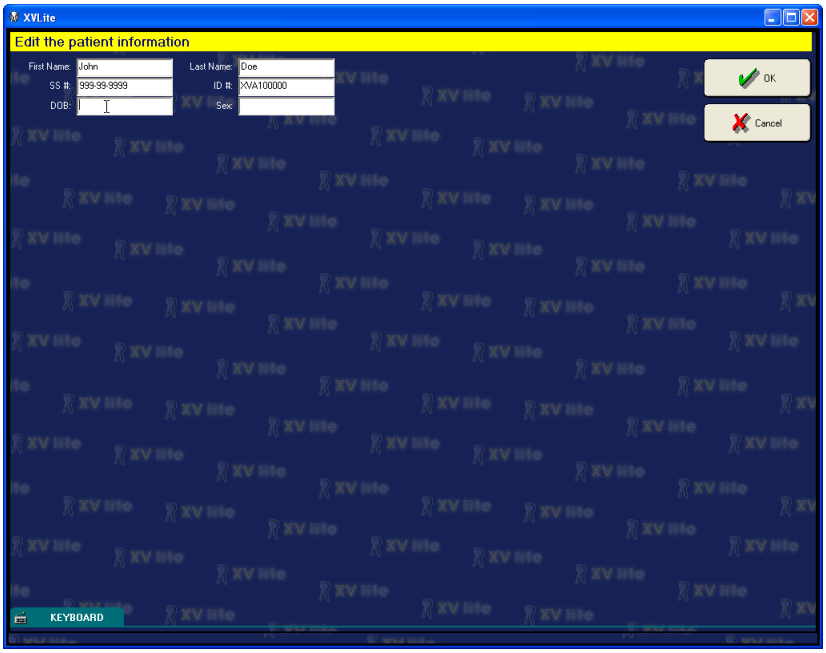

2.4 Deleting a Patient

Users can delete a patient from the database using the 'Delete Patient' function. Only one patient can be deleted at a time using this functionality.

To delete a patient:

2.4.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

2.4.2 Select the patient's record and then select **Advanced Patient Options > Delete This Patient** on the menu bar.

2.4.3 The following warning messages display. If sure, select **Yes** on each to continue with the deletion.

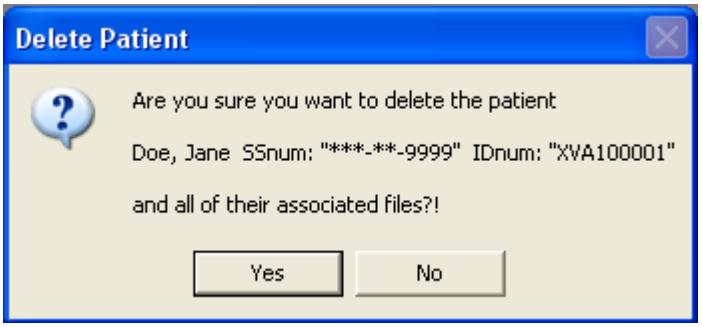
Delete Patient
Are you sure you want to delete the patient
Doe, Jane SSnum: "***-**-9999" IDnum: "XVA100001"
and all of their associated files?!
Yes
No

2.4.3.1

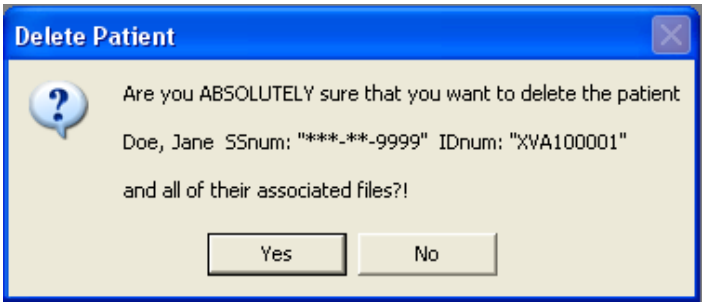
Delete Patient
Are you ABSOLUTELY sure that you want to delete the patient
Doe, Jane SSnum: "***-**-9999" IDnum: "XVA100001"
and all of their associated files?!
Yes
No

2.4.3.2

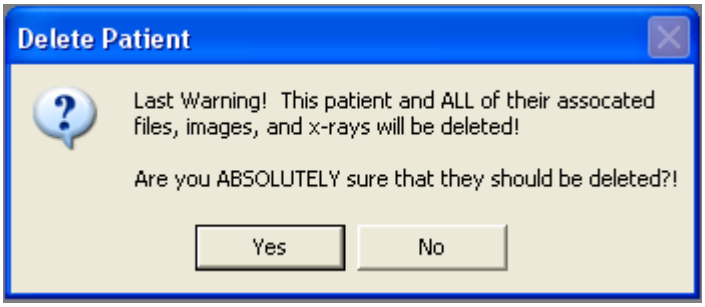
Delete Patient
Last Warning! This patient and ALL of their assocated files, images, and x-rays will be deleted!
Are you ABSOLUTELY sure that they should be deleted?!
Yes
No

2.4.3.3

2.5 Viewing an Existing Patient's Images

To view an existing patient's images:

2.5.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

2.5.2 Select the patient record and click on the **View Images** button on the menu bar.

2.5.3 The ‘View Images for which teeth?’ screen displays.

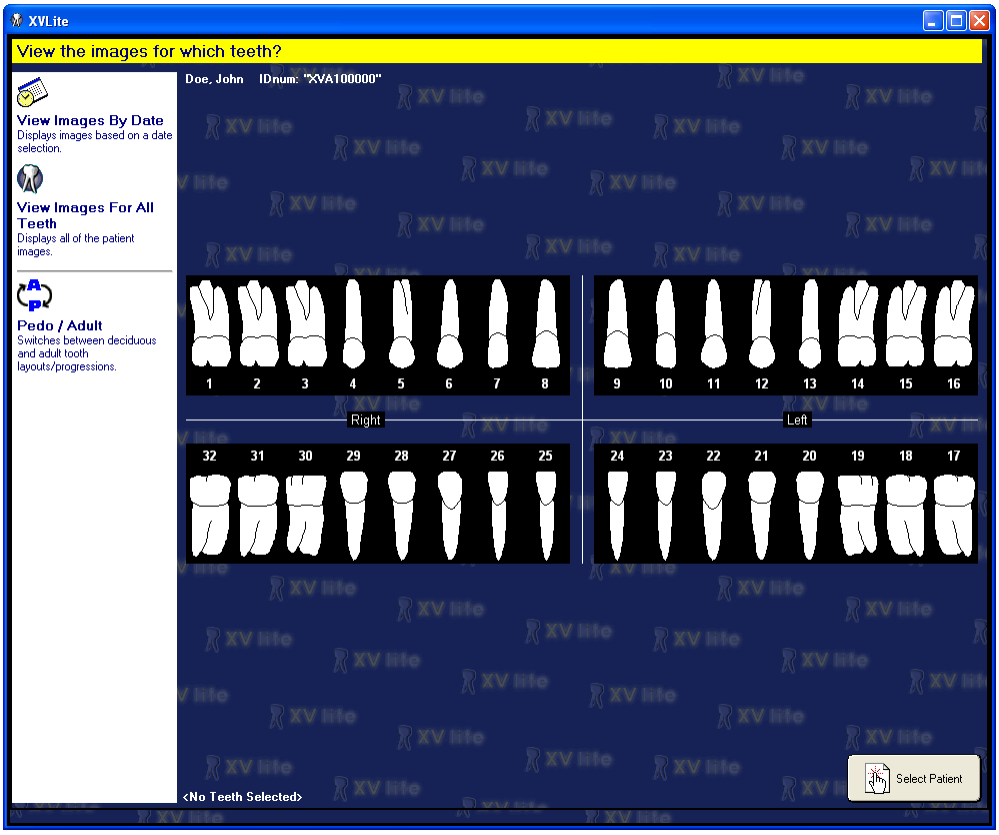
XVLite
View the images for which teeth?
Doe, John IDnum: "XVA100000"
View Images By Date
Displays images based on a date selection.
View Images For All Teeth
Displays all of the patient images.
Pedo / Adult
Switches between deciduous and adult tooth layouts/progressions.
1 2 3 4 5 6 7 8
9 10 11 12 13 14 15 16
Right
Left
32 31 30 29 28 27 26 25
24 23 22 21 20 19 18 17
<No Teeth Selected>
Select Patient

Use one of the following options to preview images of related teeth:

- **By tooth number:**
  - Click on a tooth number to view thumbnails of all images related to that tooth. Teeth with related images are displayed in white.
  - To view thumbnails of images associated to multiple teeth, left-click, hold down, and drag the cursor to select the desired teeth.
  - Click on ‘Right’ or ‘Left’ to display thumbnails of all images related to a particular side of the patient’s mouth.

- **By taken date:** Select **View Images By Date**. The wizard will progress to the 'View the images for which date?' screen. An 'All Images' collapsible list is made available to allow users to filter images by year, month, or day. Thumbnails of related images are made available for selection.

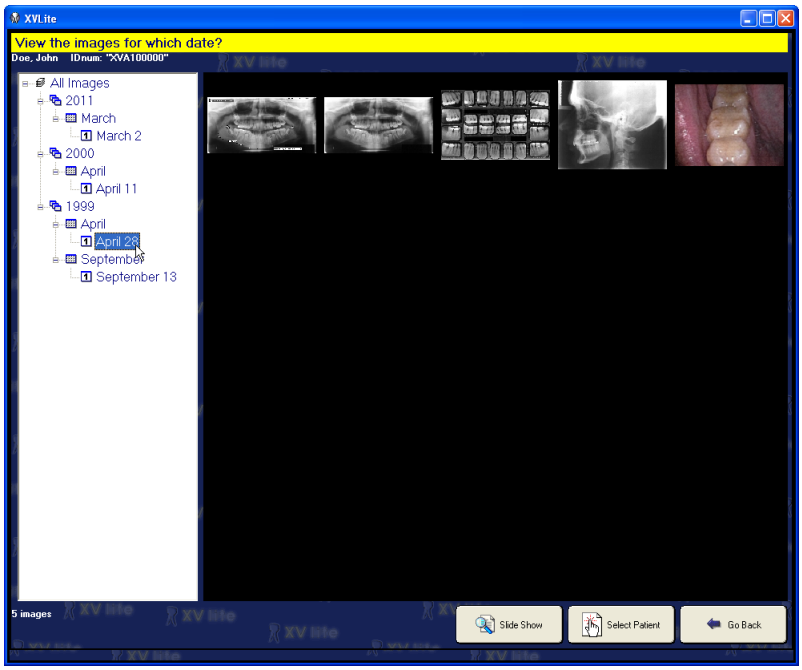

- **View All Images:** Select **View Images for All Teeth**. The wizard will progress to display thumbnails of all images in patient's database.

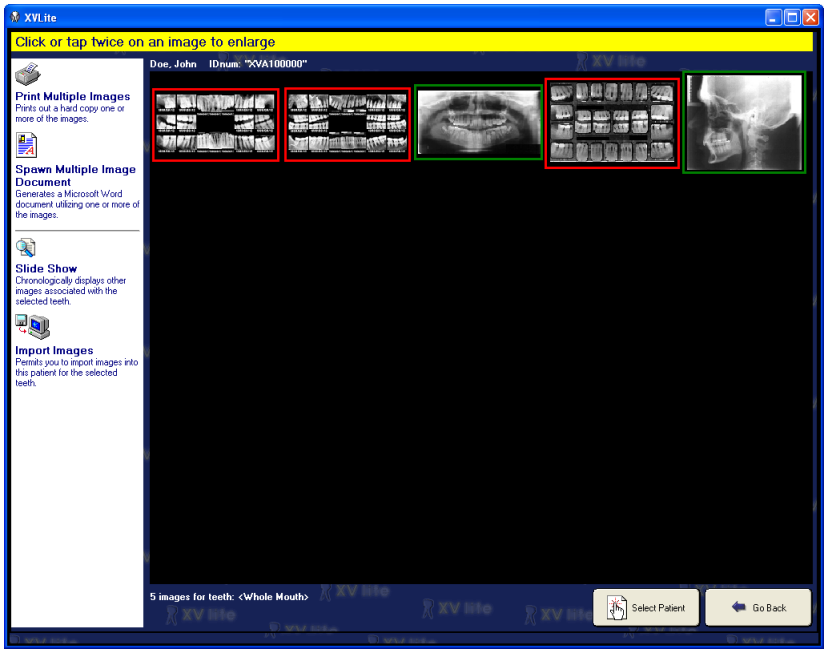
XVLite
Click or tap twice on an image to enlarge
Doe, John IDnum: "XVA100000"
Print Multiple Images
Prints out a hard copy one or more of the images.
Spawn Multiple Image Document
Generates a Microsoft Word document utilizing one or more of the images.
Slide Show
Chronologically displays other images associated with the selected teeth.
Import Images
Permits you to import images into this patient for the selected teeth.
5 images for teeth: <Whole Mouth>
Select Patient
Go Back

2.5.4 When previewing image thumbnails, the following viewing options are available:

- Double-click on any desired image layout (outlined in red) or single image thumbnail (outlined in green) to display the related image in full view.

- Select the Slide Show button to view all the related images in full view as a slideshow.

2.6 Viewing a Group/Series of Images

The imaging application has the ability to display a group of images in a single workspace known as Layouts. Layouts provide a conventional method of displaying images in the standard dental template view.

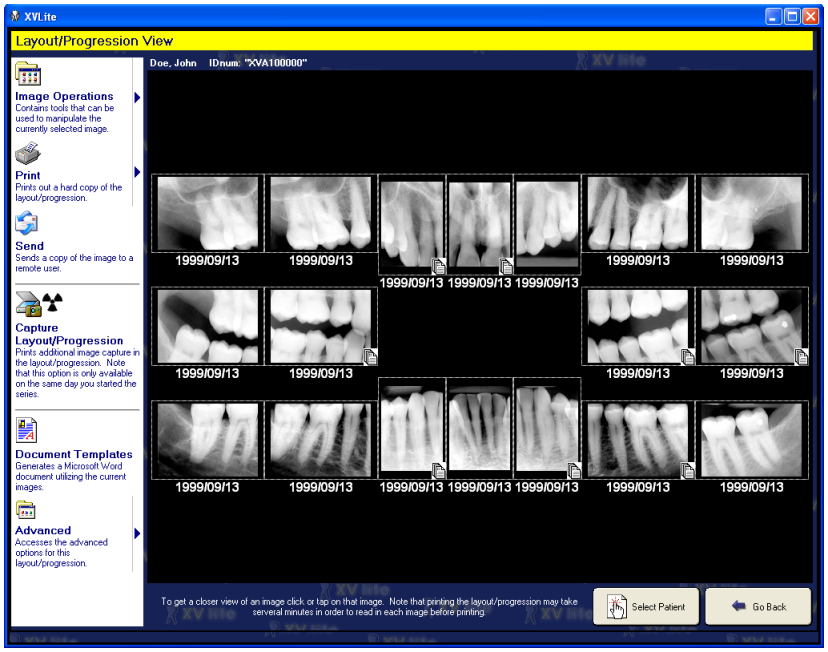
XVLite
Layout/Progression View
Doe, John IDnum: "XVA100000"
Image Operations
Contains tools that can be used to manipulate the currently selected image.
Print
Prints out a hard copy of the layout/progression.
Send
Sends a copy of the image to a remote user.
Capture Layout/Progression
Prints additional image capture in the layout/progression. Note that this option is only available on the same day you started the series.
Document Templates
Generates a Microsoft Word document utilizing the current images.
Advanced
Accesses the advanced options for this layout/progression.
1999/09/13
To get a closer view of an image click or tap on that image. Note that printing the layout/progression may take several minutes in order to read in each image before printing.
Select Patient
Go Back

Each tile in a layout identifies the related tooth associations, image orientation, and the order in the capture series however layouts can be further customized to specify the source of the image (sensor, scanner, video, etc.). Refer to Appendix B: Customizing Layout Definitions for additional information.

3 CAPTURING IMAGES FROM A X-RAY SENSOR/UNIT

3.1 Capturing Single Images from a X-ray Sensor/Unit

Take X-ray permits users to select an x-ray sensor or unit they want to use from a list of available sensors before a digital x-ray is acquired.

To capture from a sensor:

3.1.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

3.1.2 Select the patient record and click on the **Take X-ray** button on the menu bar.

3.1.3 The wizard advances to the 'Take X-rays for which teeth? …' screen. Select one or more teeth to associate to the image after the capture is complete. *This will automatically setup the tooth association with the image and properly orient the displayed image once captured.*

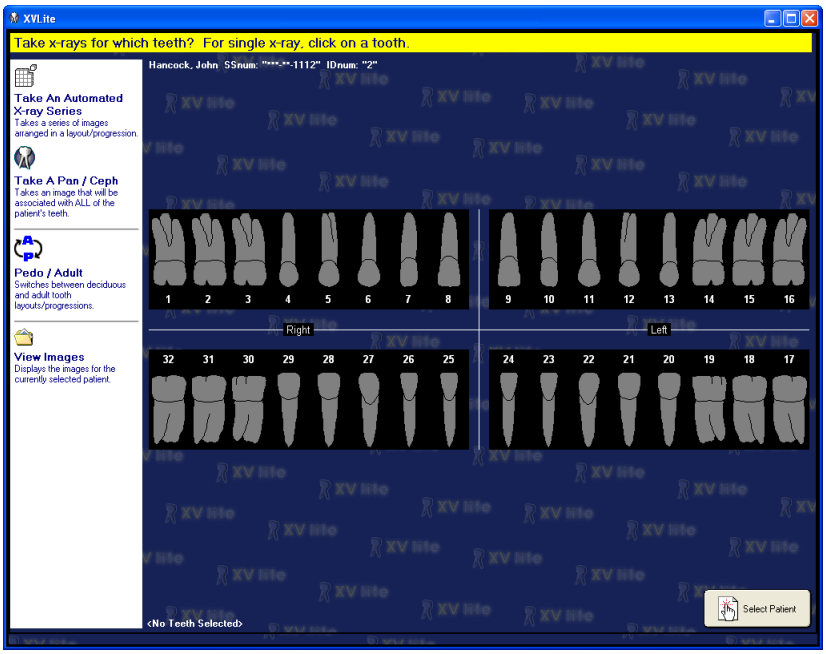
XVLite
Take x-rays for which teeth? For single x-ray, click on a tooth.
Hancock, John SSnum: "***-**-1112" IDnum: "2"
Take An Automated X-ray Series
Takes a series of images arranged in a layout/progression.
Take A Pan / Ceph
Takes an image that will be associated with ALL of the patient's teeth.
Pedo / Adult
Switches between deciduous and adult tooth layouts/progressions.
View Images
Displays the images for the currently selected patient.
1 2 3 4 5 6 7 8
9 10 11 12 13 14 15 16
Right
Left
32 31 30 29 28 27 26 25
24 23 22 21 20 19 18 17
Select Patient
<No Teeth Selected>

3.1.4 The wizard advances to the 'Position Sensor and Activate X-ray Unit' screen.

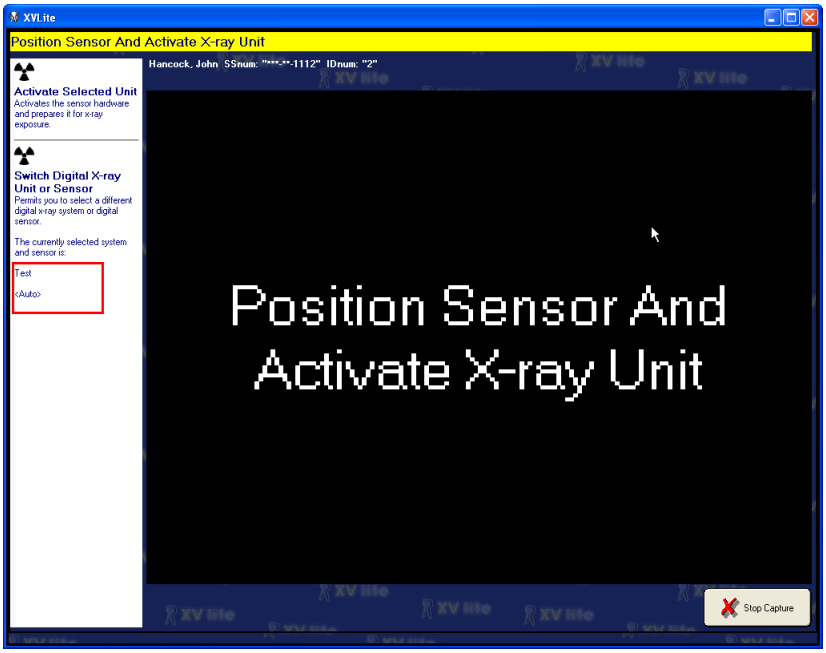
XVLite
Position Sensor And Activate X-ray Unit
Activate Selected Unit
Activates the sensor hardware and prepares it for x-ray exposure.
Switch Digital X-ray Unit or Sensor
Permits you to select a different digital x-ray system or digital sensor.
The currently selected system and sensor is:
Test
<Auto>
Position Sensor And Activate X-ray Unit
Stop Capture

3.1.5 Note that the last sensor utilized on the computer/workstation will display in the area outlined in red above. To select a different sensor, click on Switch Digital X-ray Unit or Sensor. The 'Capture Sensor Image' selection screen displays. Select the applicable sensor and then click on **OK**.

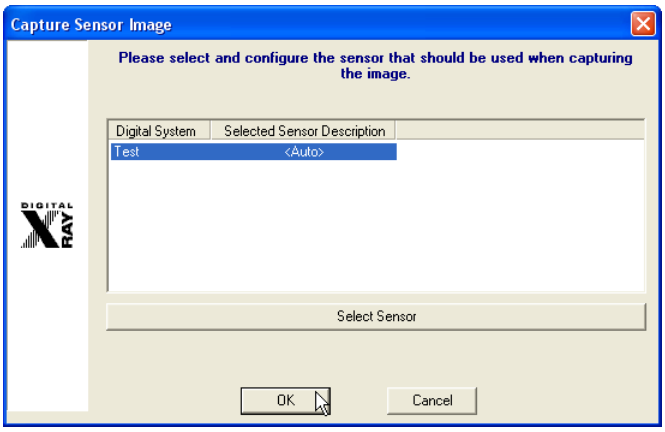

3.1.6 Click on **Activate Selected Unit** to proceed to prepare the sensor for capture. The sensor indicator will turn green when the sensor is ready to capture an image. A vocal cue will also be heard if the computer has a sound card and speakers.

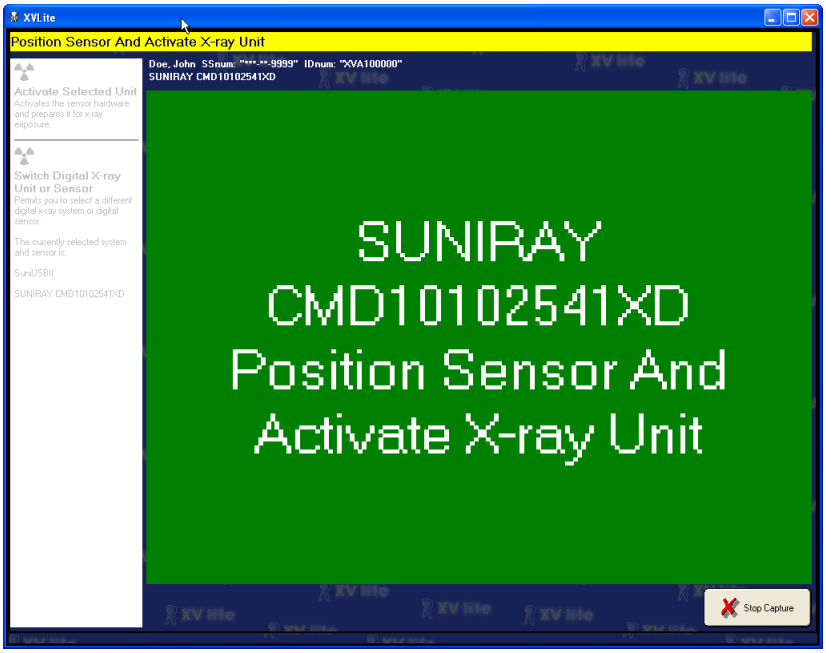
XVLite
Position Sensor And Activate X-ray Unit
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
SUNIRAY CMD10102541XD
Activate Selected Unit
Activates the sensor hardware and prepares it for x-ray exposure.
Switch Digital X-ray Unit or Sensor
Permits you to select a different digital x-ray system or digital sensor.
The currently selected system and sensor is:
SuniUSBII
SUNIRAY CMD10102541XD
SUNIRAY
CMD10102541XD
Position Sensor And
Activate X-ray Unit
Stop Capture

3.1.7 Proceed to shoot the x-ray. The new image from the sensor will be acquired and stored in the patient's record. The amount of time it takes for the image to appear on the screen is dependent upon the sensor manufacturer.

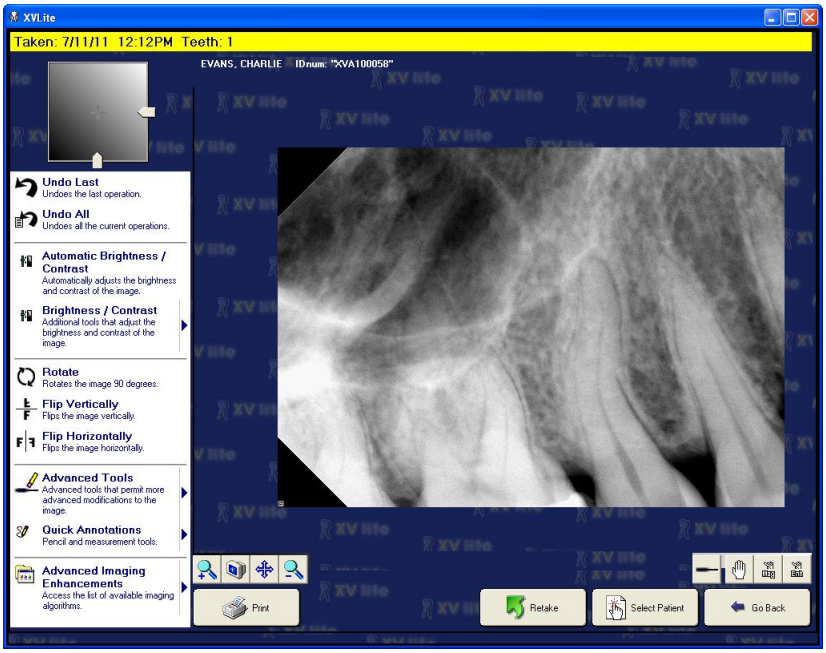

3.1.8 The image file is automatically saved and stored in the patient's file.

3.1.9 Post-capture enhancements can be applied to the newly captured image. Select **Automatic Brightness/Contrast** to have the application automatically adjust the settings … OR ... **Brightness/Contrast** to manually apply Brightness/Contrast, Equalize, Gamma Correction, or to adjust color levels.

3.1.10 Additional image enhancement utilities are available under the **Advanced Tools** menu option. Refer to the Image Enhancement section for detailed information on these and other commonly used image enhancement tools.

3.1.11 Post-capture operations can be performed on the newly captured image. Select **Rotate**, **Flip Vertically**, or **Flip Horizontally** to orient the image as desired.

3.1.12 To retake an image select the Retake button and repeat steps 3.1.7 – 3.1.11 to acquire an additional image for the teeth selected in Step 3.1.3.

3.1.13 To return to the patient list, click on the **Select Patient** button.

3.2 Capturing a Group/Layout Images from an X-ray Sensor/Unit

A layout is a group of free-floating tiles displayed in a single workspace. The groups of images can be captured and displayed in individual tiles within the selected layout.

To capture a series of images from an x-ray sensor/unit:

3.2.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

3.2.2 Select the patient record and click on the **Take X-ray** button on the menu bar. The wizard advances to the 'Take X-rays for which teeth? …' screen. Select **Take an Automated X-ray Series**.

3.2.3 The wizard will advance to a layout selection screen. Select the desired layout (2 Bite Wings, 4 Bite Wings, etc.).

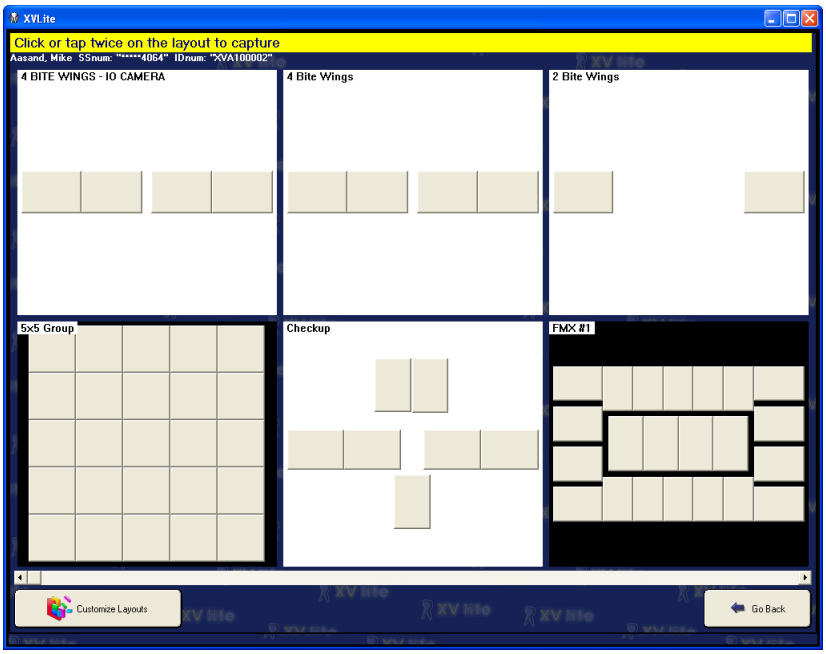

Layouts definitions specify the source (sensor, scanner, etc.) that the image will be acquire from. By default, layouts are configured to capture from sensors. If the tiles in a layout specify a source other than a Sensor it will need to be modified or a similar one created to capture from a TWAIN device or scanner. Select **Customize Layouts** and then refer to Common Layout Tasks: Changing the Capture Source (Appendix B) for detailed instructions.

3.2.4 The Wizard will advance to the Layout capture screen. Note that the first tile in the series is selected, awaiting an image capture. Additionally, note that the related tooth numbers are displayed in each tile.

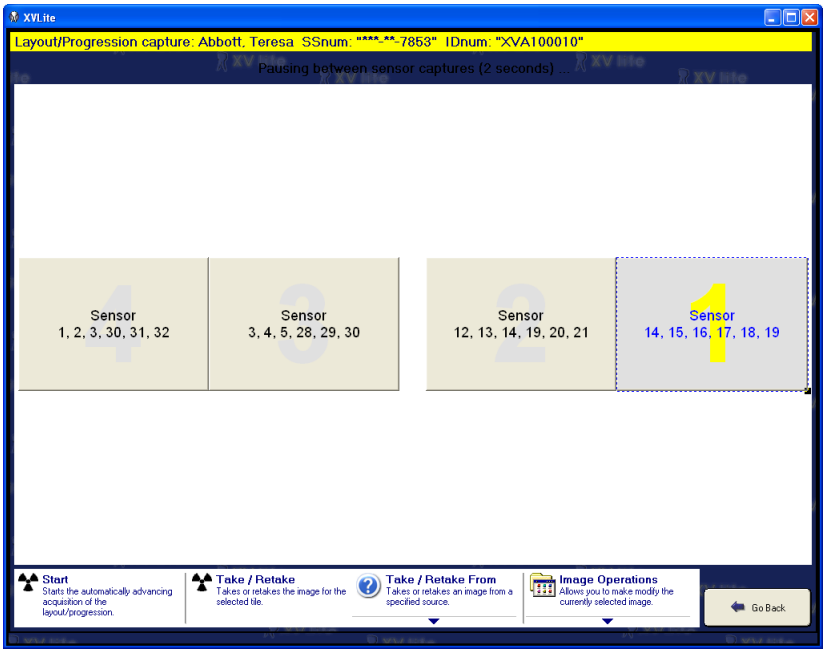
XVLite
Layout/Progression capture: Abbott, Teresa SSnum: "***-**-7853" IDnum: "XVA100010"
Pausing between sensor captures (2 seconds) ...
Sensor
1, 2, 3, 30, 31, 32
Sensor
3, 4, 5, 28, 29, 30
Sensor
12, 13, 14, 19, 20, 21
Sensor
14, 15, 16, 17, 18, 19
Start
Starts the automatically advancing acquisition of the layout/progression.
Take / Retake
Takes or retakes the image for the selected tile.
Take / Retake From
Takes or retakes an image from a specified source.
Image Operations
Allows you to make modify the currently selected image.
Go Back

Warning: X-ray images will be automatically captured in the order set by the layout definitions. They will be oriented according to the teeth defined in the layout tile. If the user deviates from the order (without taking the proper steps), images will be placed in the wrong tile and be oriented incorrectly.

3.2.5 Place the sensor in the patient's mouth and position it to capture the teeth associated to the tile. Click the **Start** button.

3.2.6 The 'Capture Sensor Image' selection screen displays. Select the applicable sensor and then click on **OK**.

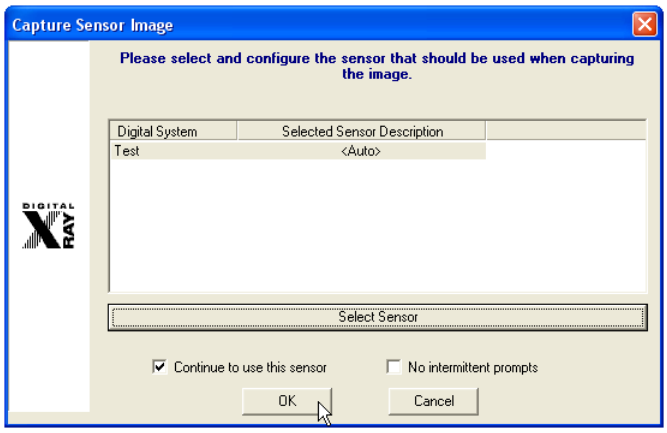

Select 'Continue to Use This Sensor' if all images in the layout will be captured using the same sensor. If unchecked, the 'Capture Sensor Image' screen will display between each capture in the series.

3.2.7 The software will advance and prepare the sensor for x-ray exposure. A green "Sensor Ready" indication will display at the top of the screen. A vocal cue will also be heard if the computer has a sound card and speakers.

3.2.8 Proceed to shoot the x-ray. The new image from the sensor will appear in the selected tile.

3.2.9 The application will then advance to the next tile in the series.

- If 'Continue using this sensor' was selected in Step 6, the sensor will automatically be prepared and readied for the next capture.
- If 'Continue using this sensor' was not selected in Step 6, the 'Capture Sensor Image' screen will display for the user to select the desired sensor. Click on OK to continue with the capture.

3.2.10 Place the sensor in the patient's mouth and position it to capture the set of teeth associated to the next tile.

3.2.11 Repeat Steps 8 – 10 until the last image in the series has been captured.

3.2.12 Click **Finished** when all images in the series are captured. The layout will be automatically stored to the patient's file.

4 CAPTURING IMAGES FROM SCANNERS

4.1 General Information

If a **TWAIN-compliant scanner** (e.g. a flatbed scanner with manufacturer-provided TWAIN drivers) is attached to the computer on which the imaging application is installed:

- The application will automatically recognize the device and configure its settings. (Before booting up Windows, turn on the power to the scanner to ensure that the computer's operating system "sees" the device).
- The scanner will available for selection in the 'Capture Image' device selection screen under the 'Scanned X-ray' (for scanning in X-rays) or 'Scanned Image' (for scanning in digital images) tabs.

If a **phosphor plate scanner** (e.g. Air Technique's ScanX®) is attached to the computer on which the application is installed:

- The application will require the related Apteryx imaging device extension to be installed in order to interface with the manufacturer's drivers.
- The scanner will be available for selection in the 'Capture Image' device selection screen under the 'Scanned X-ray' or 'Imaging Device' tabs.

In this user guide, captures will be limited to capturing from TWAIN-compliant scanners or phosphor plate scanners using the 'Scanned X-ray' tab.

4.2 Capturing Single Images from a Scanner

4.2.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

4.2.2 Select the patient record and click on the **Acquire Images** button on the menu bar.

4.2.3 The wizard advances to the 'Take X-rays for which teeth? …' screen. Select one or more teeth to associate to the image after the capture is complete. *This will automatically setup the tooth association with the image and properly orient the displayed image once captured.*

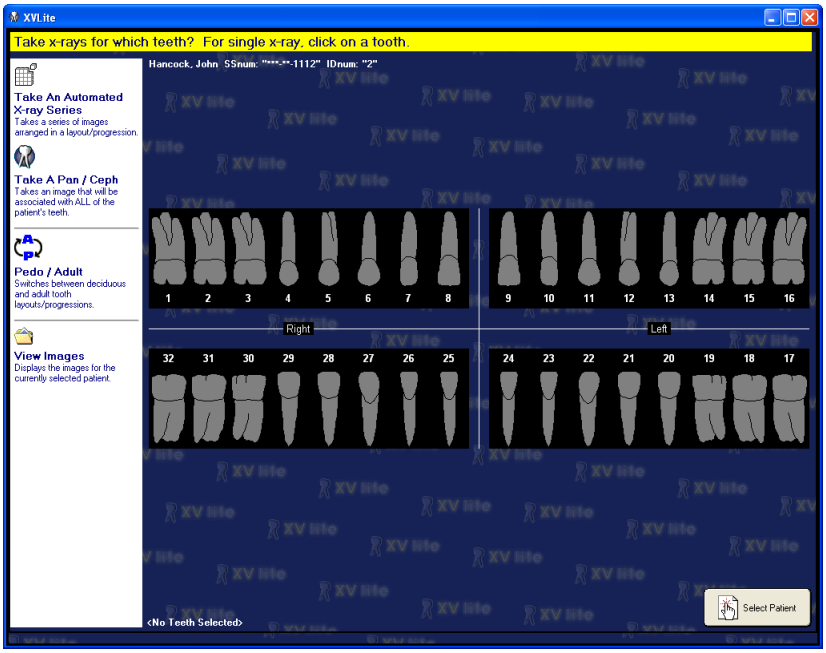
XVLite
Take x-rays for which teeth? For single x-ray, click on a tooth.
Take An Automated X-ray Series
Takes a series of images arranged in a layout/progression.
Take A Pan / Ceph
Takes an image that will be associated with ALL of the patient's teeth.
Pedo / Adult
Switches between deciduous and adult tooth layouts/progressions.
View Images
Displays the images for the currently selected patient.
1 2 3 4 5 6 7 8
9 10 11 12 13 14 15 16
Right
Left
32 31 30 29 28 27 26 25
24 23 22 21 20 19 18 17
<No Teeth Selected>
Select Patient

4.2.4 The ‘Capture Image’ device selection screen will display prompting users to select the tab that applies to the image to be captured. Select the ‘Scanned X-ray’ tab.

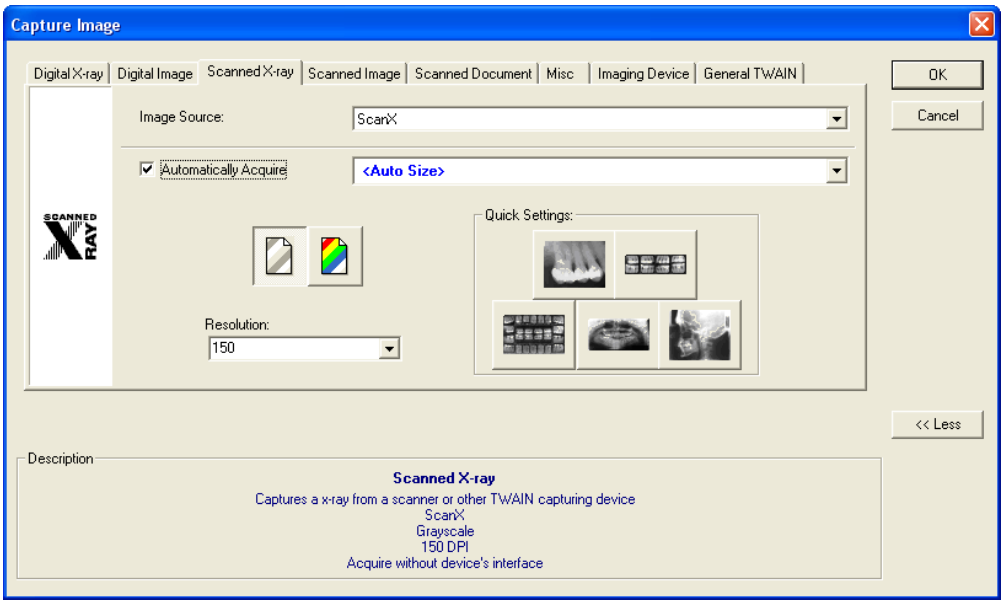

4.2.5 Click on the ‘Image Source’ drop-down list and select the applicable driver for the TWAIN-Compliant scanner or phosphor plate scanner.

4.2.6 Depending on the hardware, ‘Automatically Acquire’ may need to be disabled if a TWAIN driver is selected.

Apteryx recommends disabling ‘Automatically Acquire’ if a TWAIN driver is selected . Auto Acquire functionality depends on the capabilities of the flatbed scanner's TWAIN or Windows Imaging Acquisition (WIA) drivers. Certain scanners (such as the HP Scanjet G4050) do not work with Auto Acquire if **Auto Size** is selected, nor will they utilize the transparency adapter. If necessary, check with the hardware manufacturer to see if this functionality is supported.

4.2.6.1 If acquiring from a flatbed scanner (skip to Step 4.2.8 for phosphor plate scanners):

4.2.6.2 Place the X-ray or other media as instructed by the manufacturer.

Flatbed scanners must have a trans-illuminating cover for scanning X-rays.

4.2.6.3 Click on the **OK** button.

4.2.6.4 If this is the first time the TWAIN-compliant scanner is being used, the imaging application will display a device settings screen to configure the device. Accept the defaults by clicking the **OK** button (they can be changed at any time if necessary).

4.2.6.5 The imaging application will send instructions to the scanner and automatically scan the image and display it in the imaging application.

4.2.7 If acquiring from a phosphor plate scanner:

4.2.7.1 Click on the **OK** button. The device-specific interface will display and prompt the user when ready.

4.2.7.2 Place the X-ray film into the phosphor plate scanner as instructed by the manufacturer.

4.2.7.3 When the scan is complete, select **Done** on the device’s interface. The imaging application will then acquire the image from the device’s interface and display it in the imaging application.

4.2.8 The image file is automatically saved and stored in the patient's file.

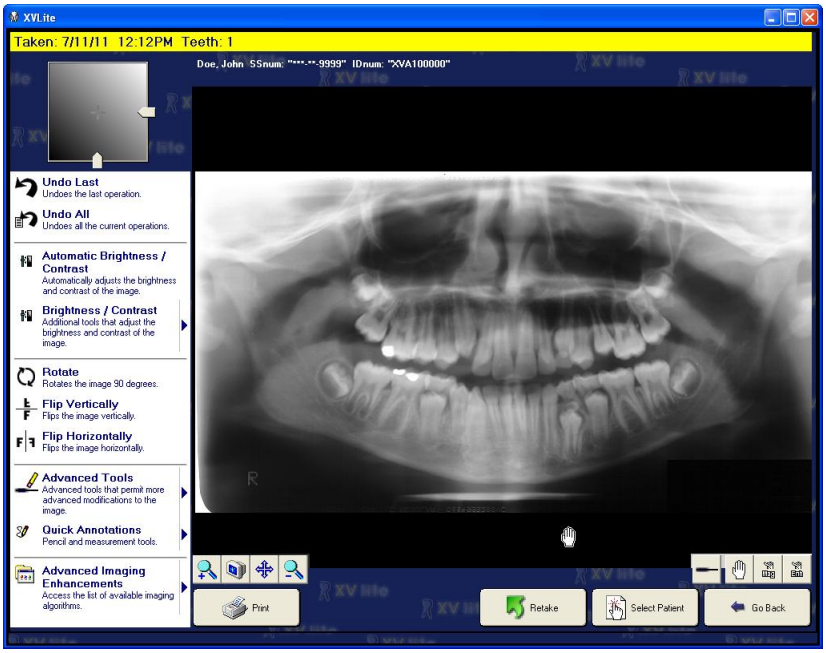

4.2.9 Post-capture enhancements can be applied to the newly captured image. Select **Automatic Brightness/Contrast** to have the application automatically adjust the settings … OR ... **Brightness/Contrast** to manually apply Brightness/Contrast, Equalize, Gamma Correction, or to adjust color levels.

4.2.10 Additional image enhancement utilities are available under the **Advanced Tools** menu option. Refer to the Image Enhancement section for detailed information on these and other commonly used image enhancement tools.

4.2.11 Post-capture operations can be performed on the newly captured image. Select Rotate, Flip Vertically, or Flip Horizontally to orient the image as desired.

4.2.12 To retake an image select the Retake button and repeat steps 4.2.7 – 4.2.11 to acquire an additional image for the teeth selected in Step 4.2.3.

4.2.13 To return to the patient list, click on the **Select Patient** button.

4.3 Capturing Group/Layout Images from Scanner

A layout is a group of free-floating tiles displayed in a single workspace. The groups of images can be captured and displayed in individual tiles within the selected layout.

To capture a series of images from a scanner:

4.3.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

4.3.2 Select the patient record and click on the **Acquire Image** button on the menu bar. The wizard advances to the 'Take X-rays for which teeth? …' screen. Select **Take an Automated X-ray Series**.

4.3.3 The wizard will advance to a layout selection screen. Select the desired layout (2 Bite Wings, 4 Bite Wings, etc.).

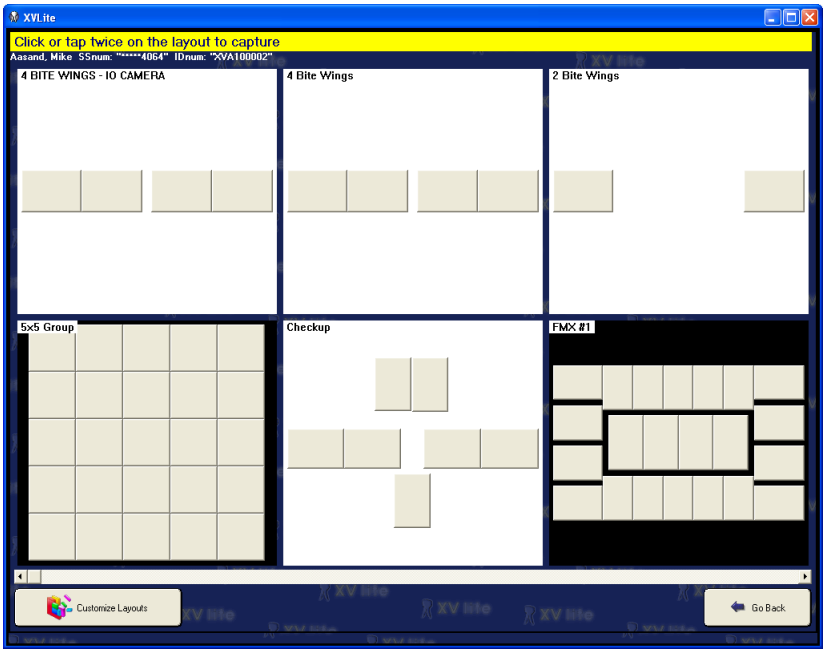

Layouts definitions specify the source (sensor, scanner, etc.) that the image will be acquire from. By default, layouts are configured to capture from sensors. If the tiles in a layout specify a source other than a TWAIN Device or "Scanner" it will need to be modified or a similar one created to capture from a TWAIN device or scanner. Select Customize Layouts and then refer to Common Layout Tasks: Changing the Capture Source (Appendix B) for detailed instructions.

4.3.4 The Wizard will advance to the Layout capture screen. Note that the first tile in the series is selected, awaiting an image capture. Additionally, note that the related tooth numbers are displayed in each tile.

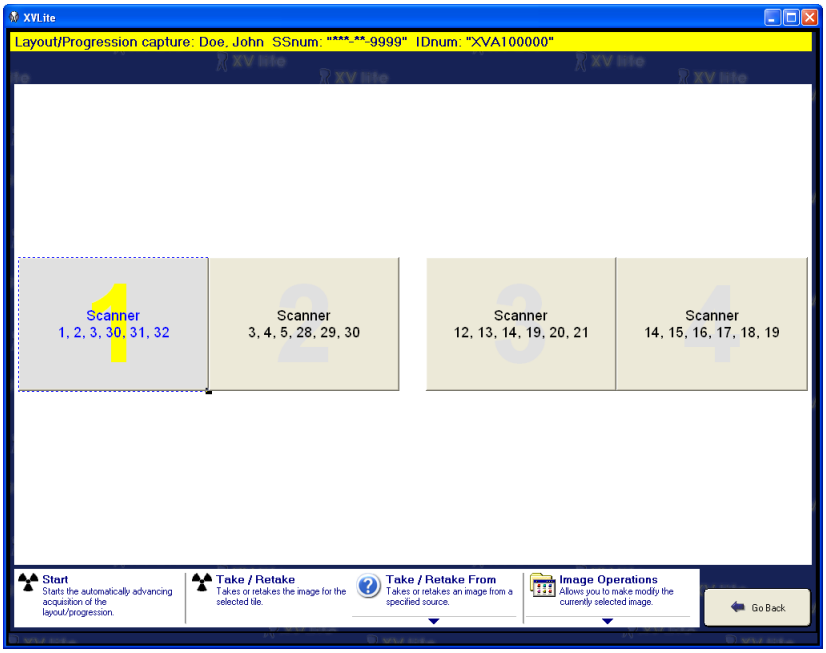

Warning: X-ray images will be automatically captured in the order set by the layout definitions. They will be oriented according to the teeth defined in the layout tile. If the user deviates from the order (without taking the proper steps), images will be placed in the wrong tile and be oriented incorrectly.

4.3.5 When ready to scan click the **Start** button.

4.3.6 The 'Capture Image' device selection screen will display prompting users to select the tab that applies to the image to be captured. Select the 'Scanned X-ray' tab.

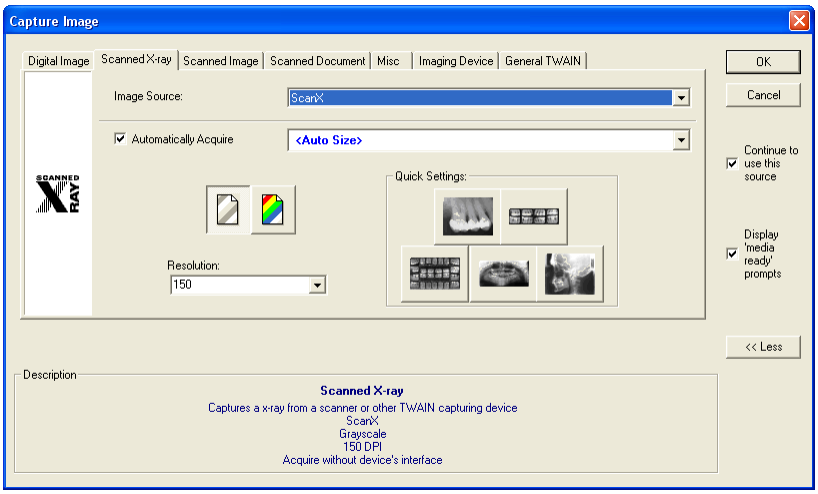

4.3.7 Click on the 'Image Source' drop-down list and select the applicable driver for the TWAIN-Compliant scanner or phosphor plate scanner.

Select 'Continue to use this source' if all images in the layout will be captured using the same device. If unchecked the 'Capture Image' screen will display between each capture in the series.

4.3.8 Depending on the hardware, 'Automatically Acquire' may need to be disabled if a TWAIN driver is selected.

Apteryx recommends disabling "Automatically Acquire if a TWAIN driver is selected. Auto Acquire functionality depends on the capabilities of the flatbed scanner's TWAIN or Windows Imaging Acquisition (WIA) drivers. Certain scanners (such as the HP Scanjet G4050) do not work with Auto Acquire if **Auto Size** is selected, nor will they utilize the transparency adapter. If necessary, check with the hardware manufacturer to see if this functionality is supported.

4.3.9 If acquiring from a flatbed scanner (skip to Step 4.3.10 for phosphor plate scanners):

4.3.9.1 Place the X-ray or other media as instructed by the manufacturer.

Flatbed scanners must have a trans-illuminating cover for scanning X-rays.

4.3.9.2 Click on the **OK** button.

4.3.9.3 If this is the first time the TWAIN-compliant scanner is being used imaging application will display a device settings screen to configure the device. Accept the defaults by clicking the **OK** button (they can be changed at any time if necessary).

4.3.9.4 The imaging application will send instructions to the scanner and automatically scan the image and display it in the selected tile.

4.3.10 If acquiring from a phosphor plate scanner:

4.3.10.1 Click on the **OK** button. The device-specific interface will display and prompt the user when ready.

4.3.10.2 Place each X-ray film into the phosphor plate scanner as instructed by the manufacturer.

4.3.10.3 When all images are scanned and display in the device interface select **Done**. The imaging application will then acquire the images from the device's interface and insert them into each tile in the capture window.

4.3.11 The application will then advance to the next tile in the series.

- If ‘Continue using this source’ was selected in Step 6, the device will automatically be prepared and readied for the next capture.
- If ‘Continue using this source’ was not selected in Step 6, the ‘Capture Image’ screen will display for the user to select the desired device from the ‘Scanned X-ray’ tab again. Click on OK to continue with the capture.

4.3.12 Repeat Steps 4.3.9.1 – 4.3.9.4 for flatbed scanners until the last image in the series has been captured.

4.3.13 Click **Finished** when all images in the series are captured. The layout will be automatically stored to the patient’s file.

5 CAPTURING IMAGES FROM AN INTRA-ORAL CAMERA

5.1 General Information

The imaging application offers an easy-to-use DirectVideo and Real-Time interface that allows users to capture live images from video sources such as Intra-Oral Cameras and digital cameras. The Real-time Video Extension is used for capturing images from older analog intra-oral video cameras connected to computers via video card. The DirectVideo Extension is more commonly used for more recent technology that connects cameras via USB, FireWire (IEEE 1394) cameras and DirectX video capture cards.

In this user guide, captures will be limited to capturing from an Intra-Oral Camera with the more commonly used DirectVideo Extension.

By default, the DirectVideo Extension is enabled. To change to Real-Time Video Extension for older, analog cameras, click on Preferences > Imaging and then select the Video Device Type button. Enable the Real-Time Video option on the 'Video Source' dialog box.

5.2 Capturing Single Images from an IO Camera

5.2.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

5.2.2 Select the patient record and click on the **Acquire Images** button on the menu bar.

5.2.3 The wizard advances to the 'Take X-rays for which teeth? …' screen. Select one or more teeth to associate to the image after the capture is complete. *This will automatically setup the tooth association with the image and properly orient the displayed image once captured.*

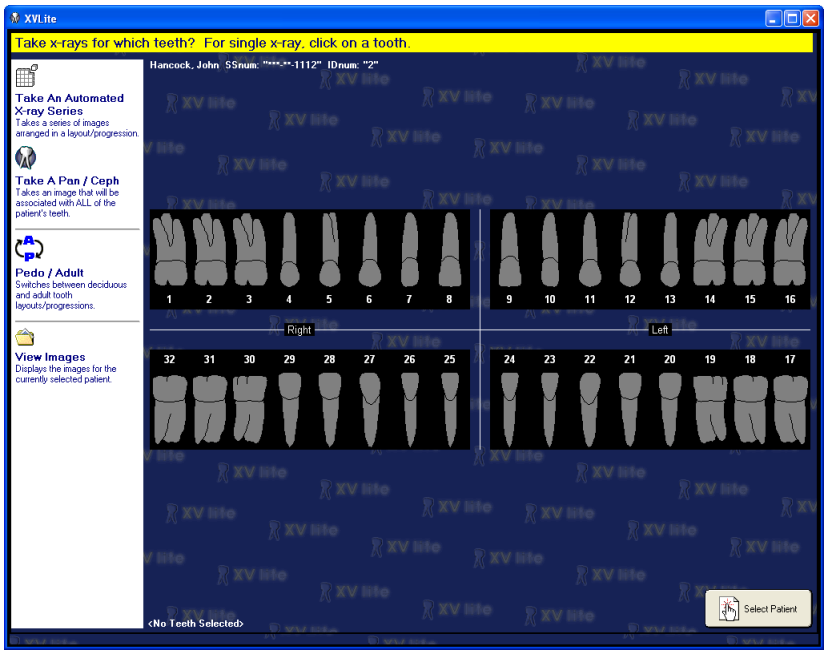
XVLite
Take x-rays for which teeth? For single x-ray, click on a tooth.
Hancock, John SSnum: "***-**-1112" IDnum: "2"
Take An Automated X-ray Series
Takes a series of images arranged in a layout/progression.
Take A Pan / Ceph
Takes an image that will be associated with ALL of the patient's teeth.
Pedo / Adult
Switches between deciduous and adult tooth layouts/progressions.
View Images
Displays the images for the currently selected patient.
1 2 3 4 5 6 7 8
9 10 11 12 13 14 15 16
Right
Left
32 31 30 29 28 27 26 25
24 23 22 21 20 19 18 17
<No Teeth Selected>
Select Patient

5.2.4 The ‘Capture Image’ device selection screen will display prompting users to select the tab that applies to the image to be captured. Select the ‘Misc’ tab

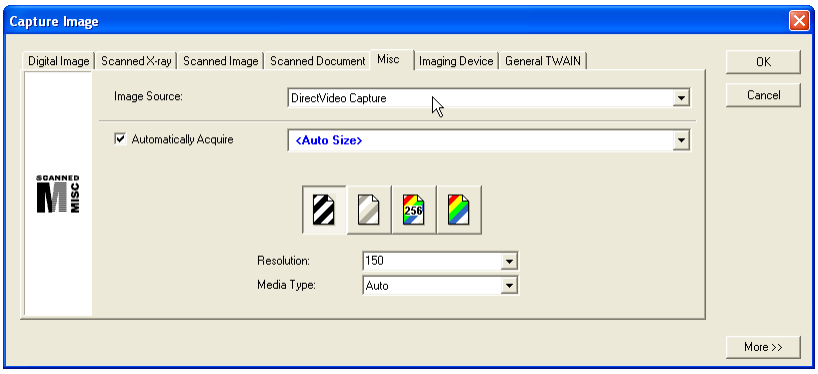

5.2.5 Click on the ‘Image Source’ drop-down list and select **DirectVideo Capture**.

5.2.6 The ‘DirectVideo’ interface displays.

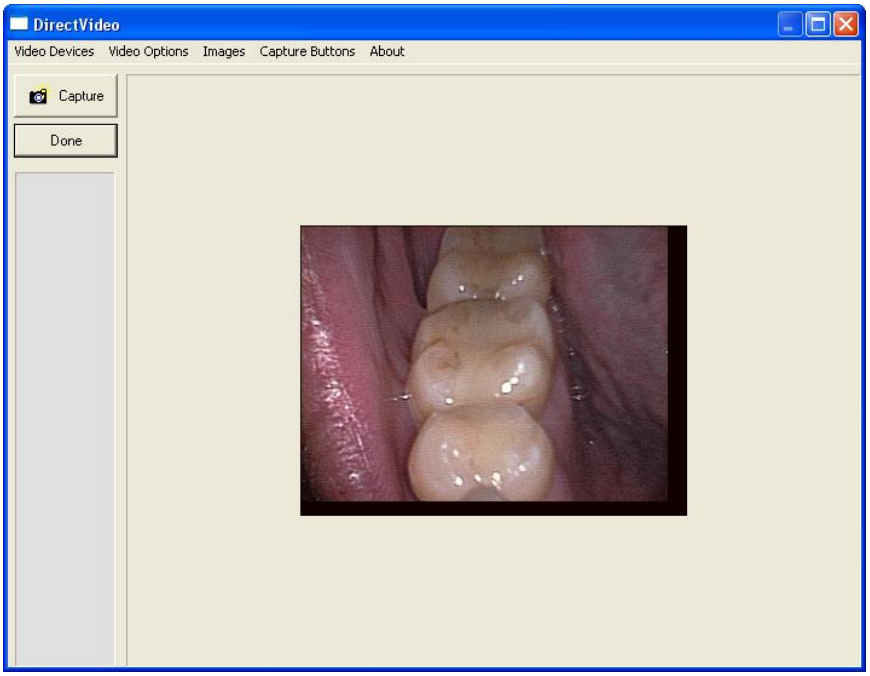

If more than one video source is attached to the computer, select Video Devices from the menu and then select the applicable device.

5.2.6.1 Note that the live video feed displays on the right hand side. Place the camera in the patient’s mouth and position it where desired.

5.2.6.2 Capture the image using one of the following methods:

- Press the button on the camera

  DirectVideo comes equipped with different capture button configurations designed to interact with various cameras. Select Camera Buttons from the menu to change the configuration to one that applies if the camera button does not trigger the capture.

- Step on the foot pedal (if configured)
- Select the **Capture** button on the ‘DirectVideo’ interface
- Press the space bar on the keyboard

5.2.6.3 Once captured, a thumbnail of the image will appear in the area below the buttons on the 'DirectVideo' interface. When finished, click the **Done** button.

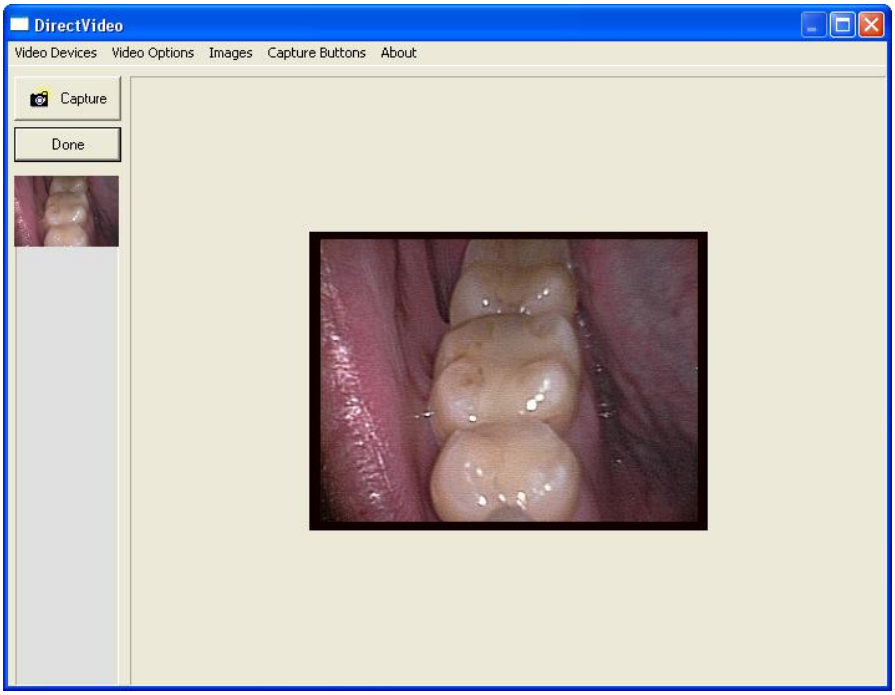

5.2.6.4 Multiple images can be captured at one time, if desired. Additional thumbnails will appear below the initial one as images are captured.

5.2.6.5 If unsatisfied with an image, right-click on the image thumbnail and select ***Delete Current Image***.

5.2.6.6 When finished, click the **Done** button.

5.2.7 The 'DirectVideo' interface will close and the image(s) will be acquired and displayed in the imaging application.

5.2.8 The image file is automatically saved and stored in the patient's file.

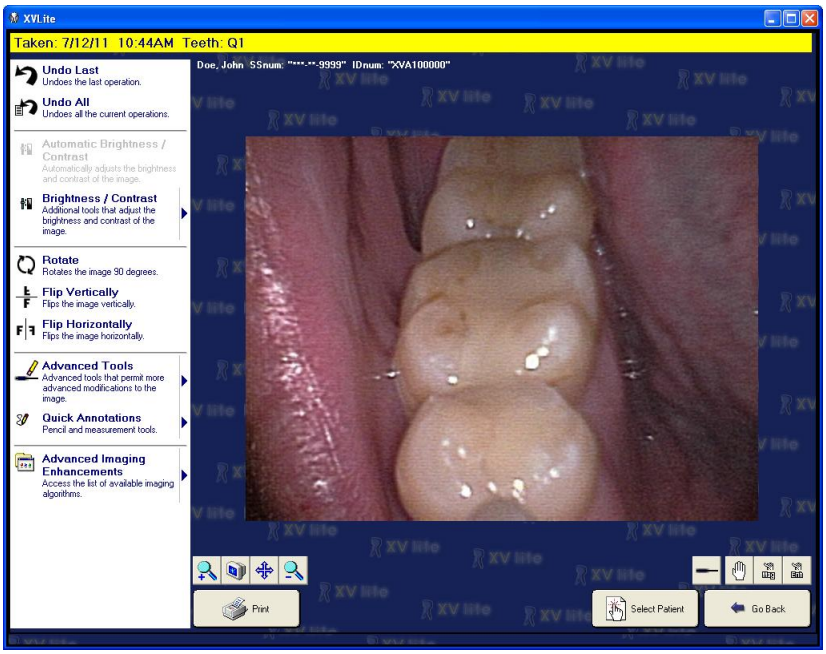

Post-capture enhancements can be applied to the newly captured image. Select Automatic Brightness/Contrast will adjust the brightness and contrast for an image automatically. The Brightness/Contrast menu contains tools that are applied manually, including: Brightness/Contrast, Equalize, Gamma Correction, or to adjust color levels.

Additional image enhancement utilities are available under the Advanced Tools menu option. Refer to the Image Enhancement section for detailed information on these and other commonly used image enhancement tools.

5.2.9 To retake an image select the Retake button and repeat steps 5.2.4 – 5.2.8 to acquire an additional image for the teeth selected in Step 5.2.3.

5.2.10 To return to the patient list, click on the **Select Patient** button.

5.3 Capturing Group/Layout Images from an IO Camera

A layout is a group of free-floating tiles displayed in a single workspace. The groups of images can be captured and displayed in individual tiles within the selected layout.

To capture a series of images from an IO camera:

5.3.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

5.3.2 Select the patient record and click on the **Acquire Image** button on the menu bar. The wizard advances to the 'Take X-rays for which teeth? …' screen. Select Take an Automated X-ray Series.

5.3.3 The wizard will advance to a layout selection screen. Select the desired layout (2 Bite Wings, 4 Bite Wings, etc.).

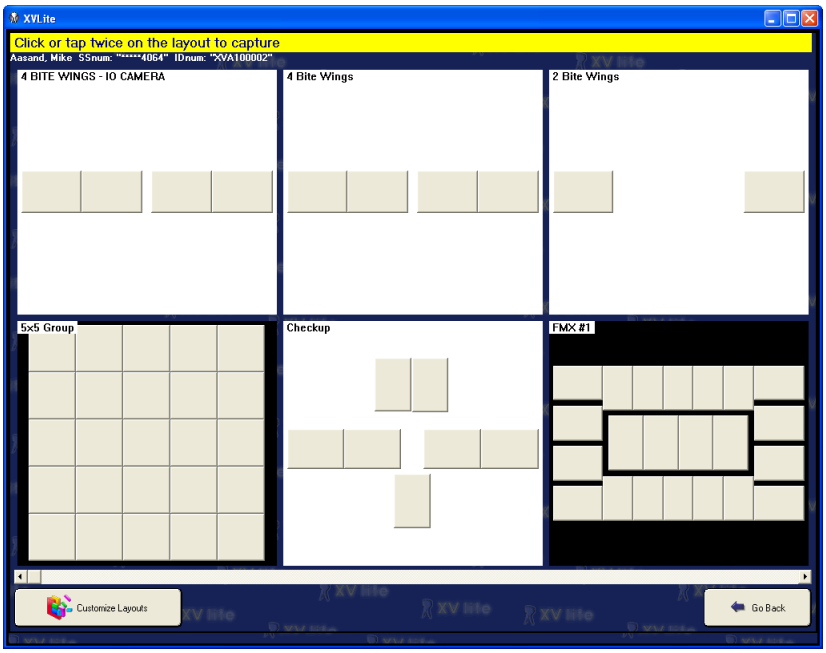

Layouts definitions specify the source (sensor, scanner, etc.) that the image will be acquire from. By default, layouts are configured to capture from sensors. If the tiles in a layout specify a source other than a Video Source it will need to be modified or a similar one created to capture from a TWAIN device or scanner. Select Customize Layouts and then refer to Common Layout Tasks: Changing the Capture Source (Appendix B) for detailed instructions.

5.3.4 The Wizard will advance to the Layout capture screen. Note that the first tile in the series is selected, awaiting an image capture. Additionally, note that the related tooth numbers are displayed in each tile.

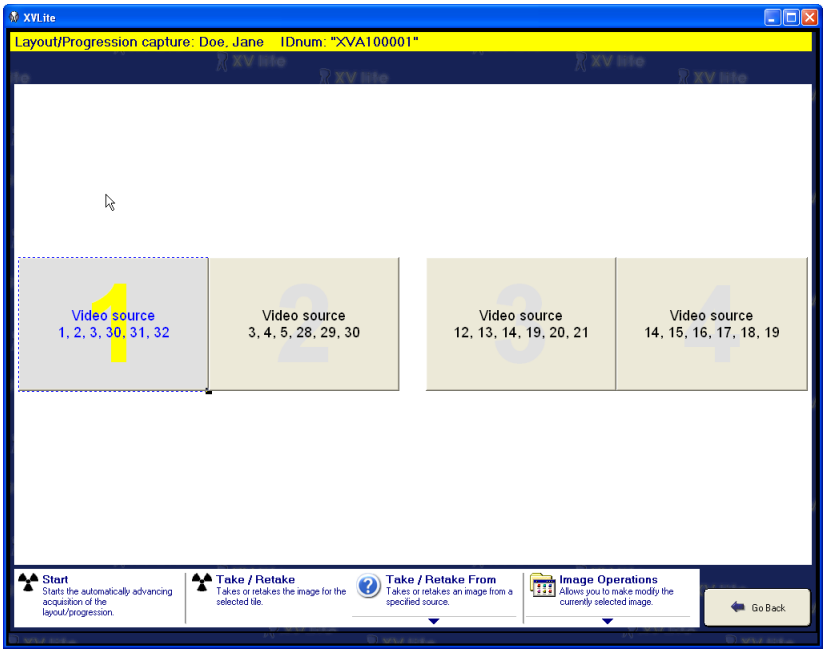
XVLite
Layout/Progression capture: Doe, Jane IDnum: "XVA100001"
Video source
1, 2, 3, 30, 31, 32
Video source
3, 4, 5, 28, 29, 30
Video source
12, 13, 14, 19, 20, 21
Video source
14, 15, 16, 17, 18, 19
Start
Starts the automatically advancing acquisition of the layout/progression.
Take / Retake
Takes or retakes the image for the selected tile.
Take / Retake From
Takes or retakes an image from a specified source.
Image Operations
Allows you to make modify the currently selected image.
Go Back

Warning: X-ray images will be automatically captured in the order set by the layout definitions. They will be oriented according to the teeth defined in the layout tile. If the user deviates from the order (without taking the proper steps), images will be placed in the wrong tile and be oriented incorrectly.

5.3.5 When ready to capture images click the **Start** button.

5.3.6 The 'DirectVideo' interface displays. Continue capturing images for each tile in the layout. Additional thumbnails will appear below the initial one as images are captured.

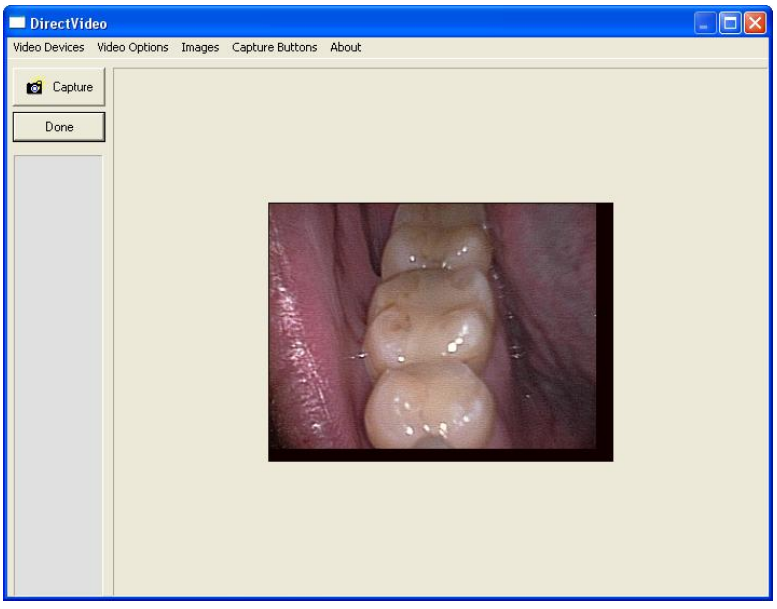

If more than one video source is attached to the computer, select Video Devices from the menu and then select the applicable device.

5.3.6.1 Note that the live video feed displays on the right hand side. Place the camera in the patient's mouth and position it where desired.

5.3.6.2 Capture the images using one of the following methods:

- Press the button on the camera
- Step on the foot pedal (if configured)
- Select the **Capture** button on the 'DirectVideo' interface
- Press the space bar on the keyboard

5.3.6.3 Once captured, a thumbnail of each image will appear in the area below the buttons on the 'DirectVideo' interface.

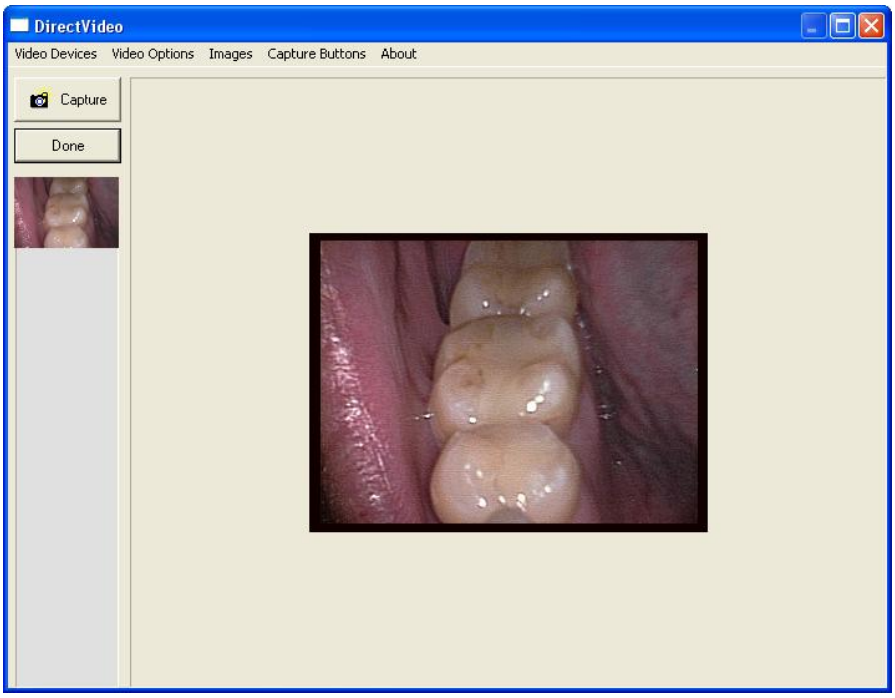

5.3.6.4 If unsatisfied with an image, right-click on the image thumbnail and select ***Delete Current Image***.

5.3.6.5 When finished, click the **Done** button.

5.3.7 The 'DirectVideo' interface will close and the images will automatically be placed in each tile in the layout.

5.3.8 Click **Finished** when all images in the series are captured. The layout will be automatically stored to the patient's file.

6 IMAGE ENHANCEMENT

6.1 General Information

The application's image manipulation and enhancement tools enables users to improve images digitally without having to re-shoot X-rays or other images. This guide will highlight the primary enhancement tools as the intuitive nature the imaging application enables the user to quickly grasp the functions and uses of the remaining tools.

6.2 Accessing Image Enhancement Options

6.2.1 View an existing patient's images and double-click to view it in full view.

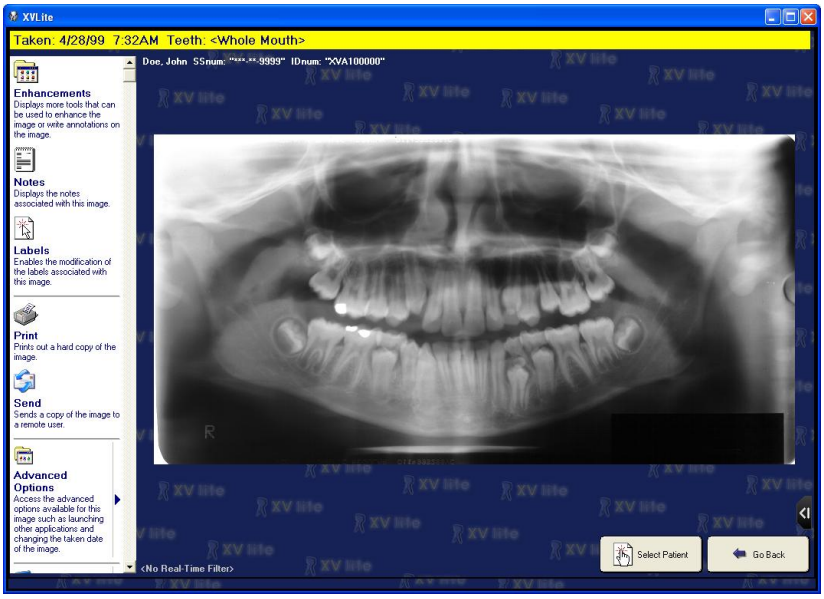
XVLite
Taken: 4/28/99 7:32AM Teeth: <Whole Mouth>
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Enhancements
Displays more tools that can be used to enhance the image or write annotations on the image.
Notes
Displays the notes associated with this image.
Labels
Enables the modification of the labels associated with this image.
Print
Prints out a hard copy of the image.
Send
Sends a copy of the image to a remote user.
Advanced Options
Access the advanced options available for this image such as launching other applications and changing the taken date of the image.
<No Real-Time Filter>
Select Patient
Go Back

6.2.2 Select **Enhancement** from the menu bar to access the image enhancement options.

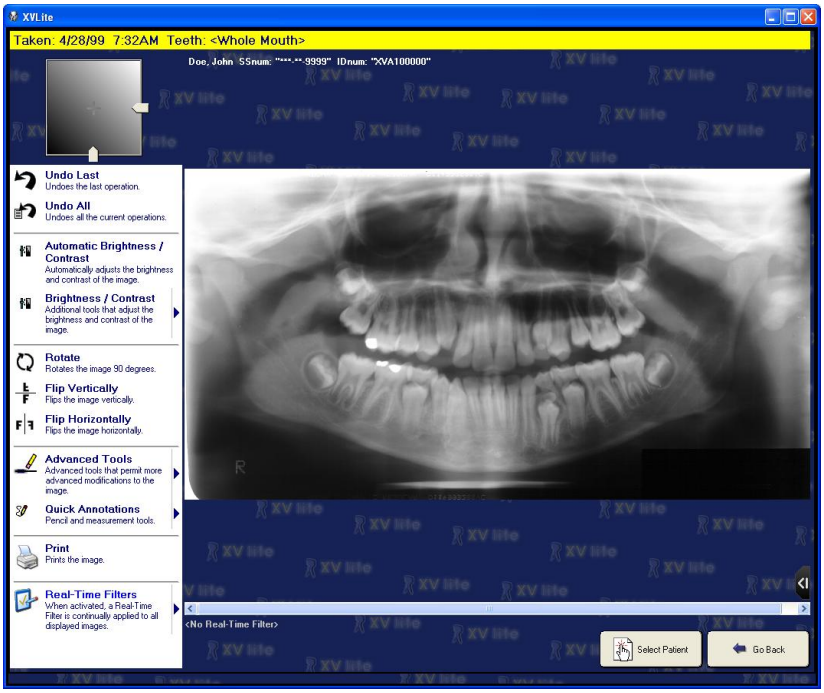
XVLite
Taken: 4/28/99 7:32AM Teeth: <Whole Mouth>
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Undo Last
Undoes the last operation.
Undo All
Undoes all the current operations.
Automatic Brightness / Contrast
Automatically adjusts the brightness and contrast of the image.
Brightness / Contrast
Additional tools that adjust the brightness and contrast of the image.
Rotate
Rotates the image 90 degrees.
Flip Vertically
Flips the image vertically.
Flip Horizontally
Flips the image horizontally.
Advanced Tools
Advanced tools that permit more advanced modifications to the image.
Quick Annotations
Pencil and measurement tools.
Print
Prints the image.
Real-Time Filters
When activated, a Real-Time Filter is continually applied to all displayed images.
<No Real-Time Filter>
Select Patient
Go Back

6.3 Brightness/Contrast

6.3.1 Overview

The imaging application provides a standard Brightness/Contrast and Gamma Correction utility that can be used to improve image quality. In general, brightness/contrast enhancement adjusts the brightness and the contrast of an image in order to try to improve the overall dynamic appearance of the image.

Gamma correction is a very versatile tool when dealing with images that are captured by video hardware. Gamma correction differs from standard brightness enhancements because it dynamically adjusts each pixel to maintain its relation to all the other pixels, hence exaggerating density changes in an object. Usually, gamma correction is used in combination with one of the other B/C enhancement tools to dramatically improve the overall appearance of an image.

Before Gamma Correction

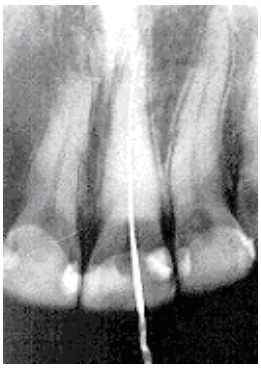

After Gamma Correction

6.3.2 Applying brightness/contrast or gamma correction

6.3.2.1 From the Enhancement menu options, select **Brightness / Contrast > Brightness / Contrast** or **Brightness / Contrast > Gamma Correction**. The applicable dialog box displays.

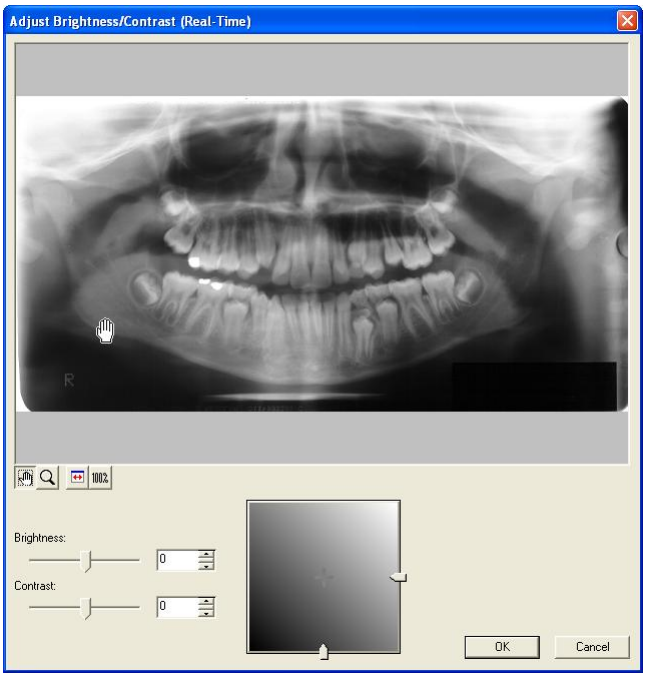

6.3.2.2 Use one of the following image adjustment buttons to size, resize, or reposition the images displayed in the original and resulting image preview windows as desired:

- - Select to pan the image in the preview to view a specific area. Click and drag the image with the left mouse button.
- - Select to magnify or reduce the image in the preview. To increase the magnification of an image, click on the image in the preview with the left mouse button. To reduce the magnification, click with the right mouse button.
- - Select to automatically resize the image and make it fit in the viewing area.
- - Select to automatically resize the image in the preview to 100% magnification. When clicked, the image in the preview will resize to the actual dimensions of the image.

6.3.2.3 Use the brightness and contrast sliders … OR … click and drag the sliders located on the right side (brightness) and bottom (contrast) of the adjustment tool to enhance the image as desired. The enhancements are adjusted in real-time in the 'Resulting Image Preview' area.

6.3.2.4 Click **OK** to apply the settings to the image.

6.3.2.5 If desired, click on Undo ( ) to remove the B/C enhancement applied to the image.

6.3.2.6 When done, click **Go Back** to return to the patient images or **Select Patient** to return to the patient list. A dialog box will appear prompting the user to save the modification. Select **Yes** to save the change.

6.3.3 Applying Equalization

The imaging application offers users the ability to apply equalization by selecting **Brightness / Contrast > Equalize**. Equalize provides a non-linear approach to altering the brightness/contrast of an image. This enhancement is typically used to improve the image quality of very low contrast images.

Most images span an entire range of brightness with all levels well represented. However, sometimes images are too light or too dark and some levels are overpopulated leaving others under-populated. The Equalize effect modifies an image so that all levels of brightness are equally well represented within the image. The equalize option is only available for grayscale images.

Before Equalization

After Equalization

6.4 Sharpening

6.4.1 Overview

Most images have some degree of blurriness (from focus problems or inherent limitations in the image taking process). The imaging application offers an automatic image sharpening that can be applied to compensate for the blurriness in an image.

Before Laplace Edge Enhancement

After Laplace Edge Enhancement

6.4.2 Applying sharpening or Laplace edge enhancement

6.4.2.1 Select **Advanced Tools > Sharpening** to use the sharpening. The 'Sharpen Image' dialog box displays.

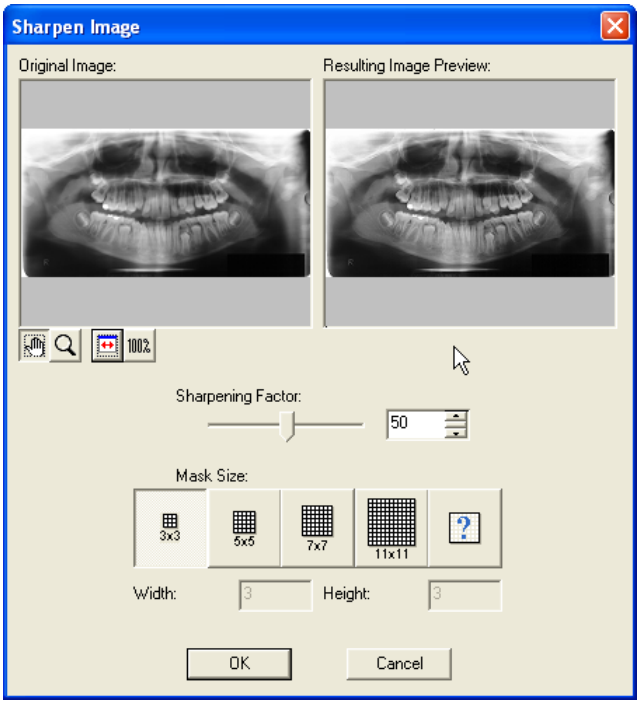

6.4.2.2 Use one of the following image adjustment buttons to size, resize, or reposition the images displayed in the original and resulting image preview windows as desired:

- - Select to pan the image in the preview to view a specific area. Click and drag the image with the left mouse button.
- - Select to magnify or reduce the image in the preview. To increase the magnification of an image, click on the image in the preview with the left mouse button. To reduce the magnification, click with the right mouse button.

- - Select to automatically resize the image and make it fit in the viewing area.
- - Select to automatically resize the image in the preview to 100% magnification. When clicked, the image in the preview will resize to the actual dimensions of the image.

6.4.2.3 The mask size and sharpening factor work hand-in-hand in determining the degree of sharpening that is applied to the image.

6.4.2.4 The 'Sharpening Factor' specifies the magnitude of the sharpening operation. Use the slider to manually adjust the degree of image sharpening as desired.

6.4.2.5 Select a predefined 'Mask Size' … OR … select to manually enter a custom 'Width' and 'Height'. The mask size specifies how large the area should be when sharpening a portion of the image. The larger the area, the wider the blurriness is considered to be.

6.4.2.6 Click **OK** to apply the settings to the image.

6.4.2.7 When done, click **Go Back** to return to the patient images or **Select Patient** to return to the patient list. A dialog box will appear prompting the user to save the modification. Select **Yes** to save the change.

6.5 Noise Removal

6.5.1 Overview

Noise in an image can be caused by a number of factors such as dust, scratches or image static. A median noise removal/reduction algorithm is provided in the imaging application. In most cases, median noise reduction results in the best image quality. It is important to note that excessive noise reduction leads to a loss of detail.

Before Noise Removal

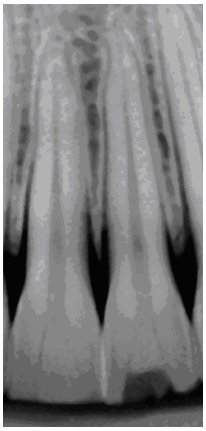

After Noise Removal

6.5.2 Applying Median Noise Removal

6.5.2.1 Select **Advanced Tools > Remove Noise**. The 'Noise Reduction (Median)' dialog box displays.

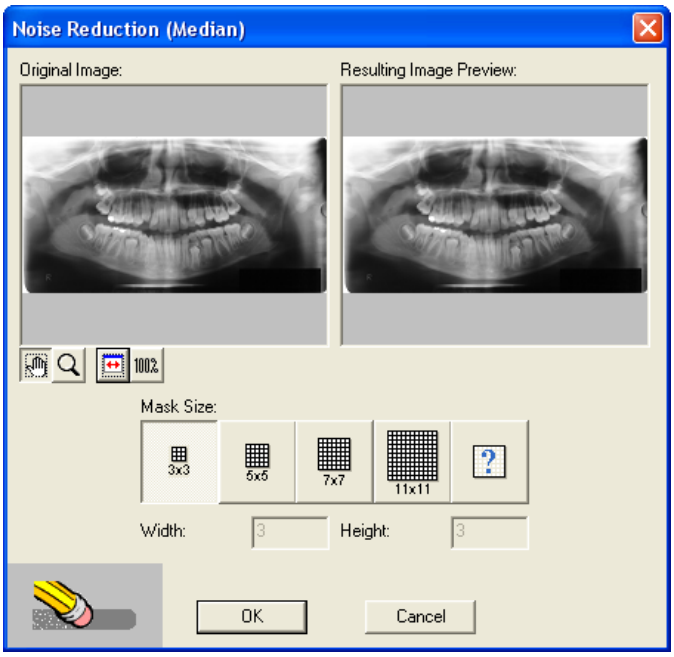

6.5.2.2 Use one of the following image adjustment buttons to size, resize, or reposition the images displayed in the original and resulting image preview windows as desired:

- - Select to pan the image in the preview to view a specific area. Click and drag the image with the left mouse button.
- - Select to magnify or reduce the image in the preview. To increase the magnification of an image, click on the image in the preview with the left mouse button. To reduce the magnification, click with the right mouse button.
- - Select to automatically resize the image and make it fit in the viewing area.
- - Select to automatically resize the image in the preview to 100% magnification. When clicked, the image in the preview will resize to the actual dimensions of the image.

6.5.2.3 Select a predefined 'Mask Size' … OR … select to manually enter a custom 'Width' and 'Height'. The mask size specifies how large the area should be when sharpening a portion of the image. The larger the area, the wider the area of noise is considered to be.

6.5.2.4 Click **OK** to apply the settings to the image.

6.5.2.5 When done, click **Go Back** to return to the patient images or **Select Patient** to return to the patient list. A dialog box will appear prompting the user to save the modification. Select **Yes** to save the change.

6.6 Real-Time Filters

Real-Time Filters are sets of image enhancements applied to any image that is opened, but the enhancement is not saved upon the image thus preserving the authentic image. Accordingly, the filters can be turned on and off. Apteryx, Inc. provides several default Real-Time Filters that can be applied to obtain different results.

Even though various workstations can apply their own real-time filters, the images in the shared database are not modified when closed.

6.6.1 Enabling or disabling a Real-Time Filter

6.6.1.1 View a layout/progression or image and select **Real-Time Filters** and choose from the following options:

- **Apteryx General Enhancement** – By default, applies Normalize; Median Blur (5x5 Mask Size); and Sharpen (21x21 Mask Size); and Gamma Correction. These options may be modified by accessing the Image Filter Options.
- **Custom Image Enhancement** – By default, applies a Median Filter (3x3 Mask Size); Sharpen (7X7 Mask Size); Adaptive Normalize; and Gamma Correction. These options may be modified by accessing the Image Filter Options.
- **General Endo Enhancement** – Applies Adaptive Normalize (1,1), Sharpen (mask size varies on the size of the image), Gamma (.7,.7,.7), Median Noise Removal, Adjust Levels (0,128,225) .
- **None** – Turns off the Real-Time Filter feature to display unfiltered, raw images.

6.6.1.2 Once selected, the bottom of the imaging application will indicate that the Real-Time Filter is enabled.

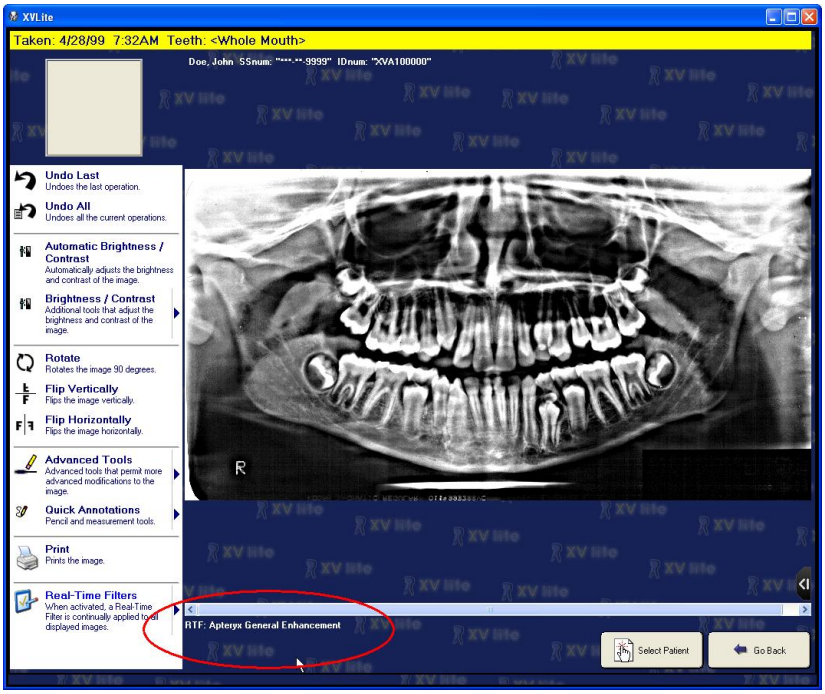
XVLite
Taken: 4/28/99 7:32AM Teeth: <Whole Mouth>
Undo Last
Undoes the last operation.
Undo All
Undoes all the current operations.
Automatic Brightness / Contrast
Automatically adjusts the brightness and contrast of the image.
Brightness / Contrast
Additional tools that adjust the brightness and contrast of the image.
Rotate
Rotates the image 90 degrees.
Flip Vertically
Flips the image vertically.
Flip Horizontally
Flips the image horizontally.
Advanced Tools
Advanced tools that permit more advanced modifications to the image.
Quick Annotations
Pencil and measurement tools.
Print
Prints the image.
Real-Time Filters
When activated, a Real-Time Filter is continually applied to all displayed images.
RTF: Apteryx General Enhancement
Select Patient
Go Back

6.6.2 Adjusting Real-Time Filter Options

The imaging application provides the ability to adjust the default settings of various image real-time filter options.

To modify a real-time filter:

6.6.2.1 Select **Real-Time Filters > Image Filter Options** and choose the applicable real-time filter option to modify.

6.6.2.2 The filter's 'Enhance Options' dialog box displays. Modify any of the available settings as needed and then click **OK**.

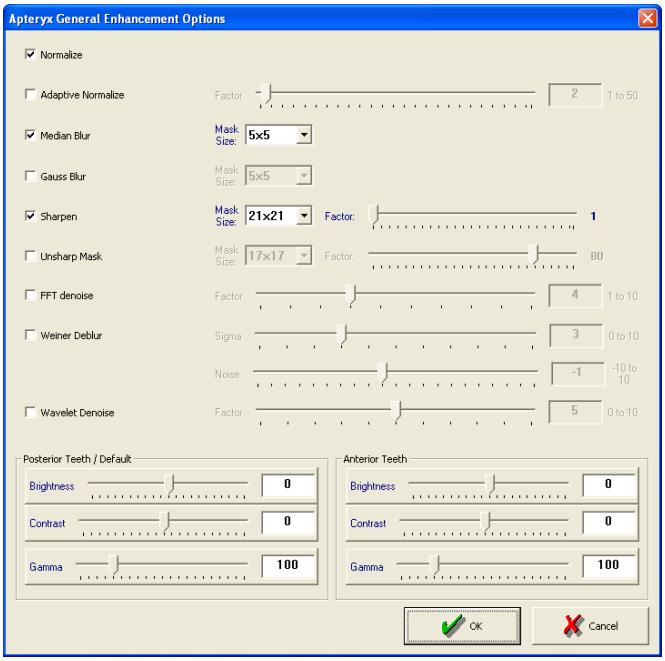

7 LABELLING IMAGES

7.1 General Information

Unlike other systems, the imaging application provides users with a set of temporary labels (marker and annotations) that can be associated with an image. A variety of different labels, markers and annotations can be applied to an image to highlight problem areas, add date and time information, define and identify earlier procedures performed, or add general notes.

Labels are not part of the image when added. They are floating objects that can be moved, modified, resized or deleted at any time.

7.2 Adding and Modifying Labels, Markers and Annotations

The following example of how to add an Ellipse to an image effectively demonstrates how to add other types of labels, markers, and annotations available in the imaging application.

The Ellipse Label command will place an ellipse on an image. Placing an ellipse on an image is useful in bringing attention to a designated area. Users have control of the ellipse's properties.

7.2.1 View an existing patient's images and double-click to view it in full view.

XVLite
Taken: 4/1/11 3:07PM Teeth: 1
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Notes
Displays the notes associated with this image.
Labels
Enables the modification of the labels associated with this image.
Print
Prints out a hard copy of the image.
Send
Sends a copy of the image to a remote user.
Document Templates
Generates a Microsoft Word document utilizing the current images.
Advanced Options
Access the advanced options available for this image such as launching other applications and changing the taken date of the image.
Select Patient
Go Back

7.2.2 Select ***Labels*** from the menu bar to access the labeling options.

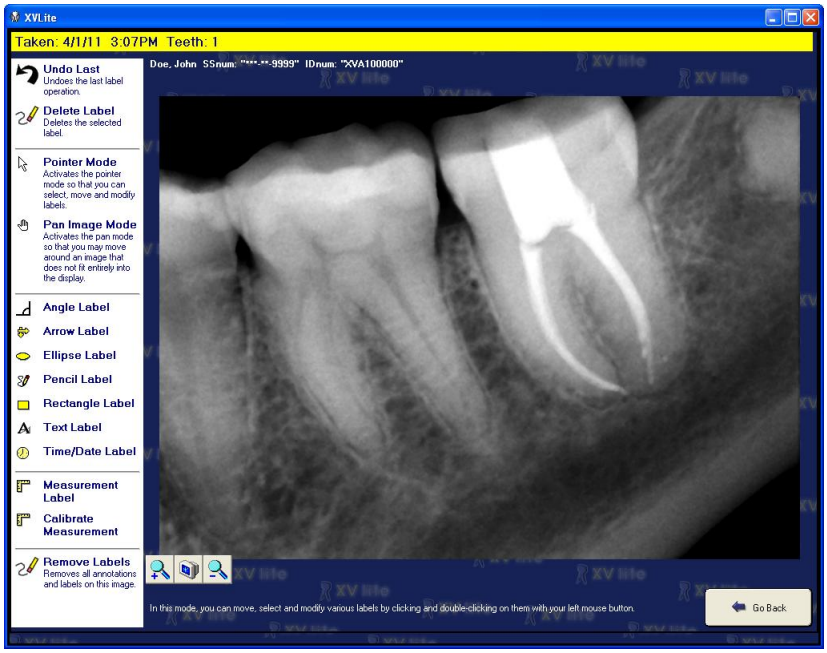
XVLite
Taken: 4/1/11 3:07PM Teeth: 1
Undo Last
Undoes the last label operation.
Delete Label
Deletes the selected label.
Pointer Mode
Activates the pointer mode so that you can select, move and modify labels.
Pan Image Mode
Activates the pan mode so that you may move around an image that does not fit entirely into the display.
Angle Label
Arrow Label
Ellipse Label
Pencil Label
Rectangle Label
Text Label
Time/Date Label
Measurement Label
Calibrate Measurement
Remove Labels
Removes all annotations and labels on this image.
In this mode, you can move, select and modify various labels by clicking and double-clicking on them with your left mouse button.
Go Back

7.2.3 Select ***Ellipse*** Label from the menu bar.

7.2.4 Hover the cursor over the image and note that it changes into a cross-hair indicator.

7.2.5 Place the stem of the indicator in the desired position on the image, Click and drag the mouse to the position where the label should be displayed. Release the mouse button to place the label in the designated location.

7.2.6 Double-click on the label to access the 'Ellipse Properties' dialog box:

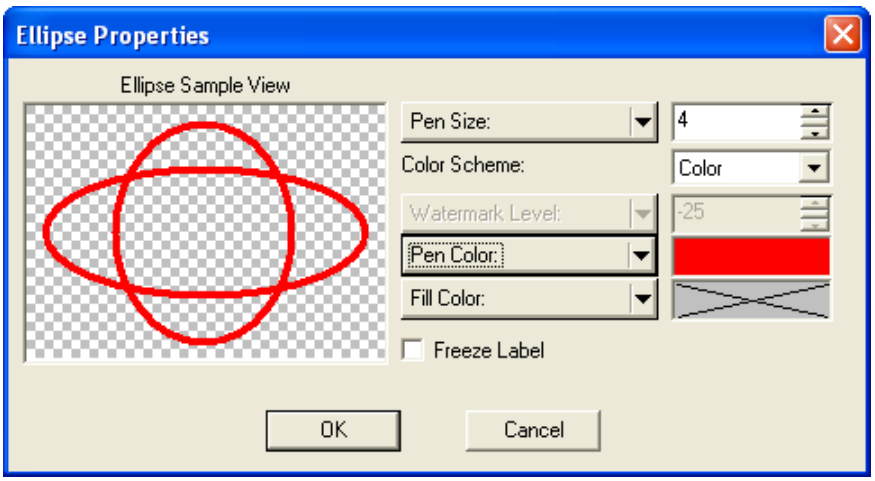

7.2.6.1 Select the desired 'Pen Size', 'Pen Color', and 'Fill Color'.

7.2.6.2 If desired, select 'Freeze Label' on the bottom-left of the dialog box to fix the position of the label. The label will not be able to be moved around on the image.

7.2.6.3 When satisfied, click on **OK**.

7.2.7 The modified properties will then be applied to label.

7.3 Calibrating Images and Adding Measurement Labels

7.3.1 Overview

Before measurements are added in an image, the image should first be calibrated. In general, images are calibrated by taking a measurement of an object of a known size or length in an image (as shown in the image below) and then providing the actual length or size of the object to determine the images calibration factor for a subsequent measurement to be performed. This method is useful in calibrating images from Cephalometric systems.

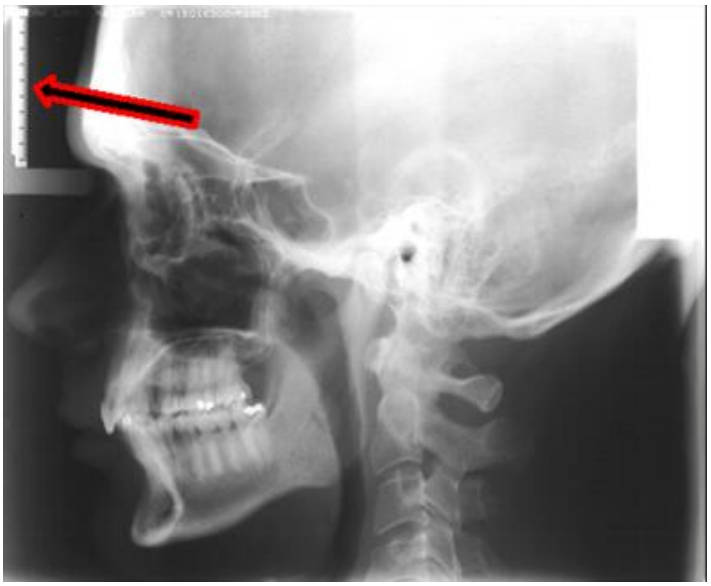

Sensor images can be more accurately calibrated by using the actual dimensions of the sensor's active area rather than an object of known length. The active area of the sensor can be determined by referring to the hardware's documentation or contacting the manufacturer.

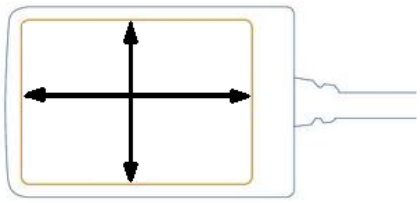

Apteryx, Inc. does not guarantee the accuracy of any calibration/measurement performed in the imaging application.

7.3.2 Calibrating an Image

The Ellipse Label command will place an ellipse on an image. Placing an ellipse on an image is useful in bringing attention to a designated area. Users have control of the ellipse's properties.

7.3.2.1 View an existing patient's images and double-click to view it in full view.

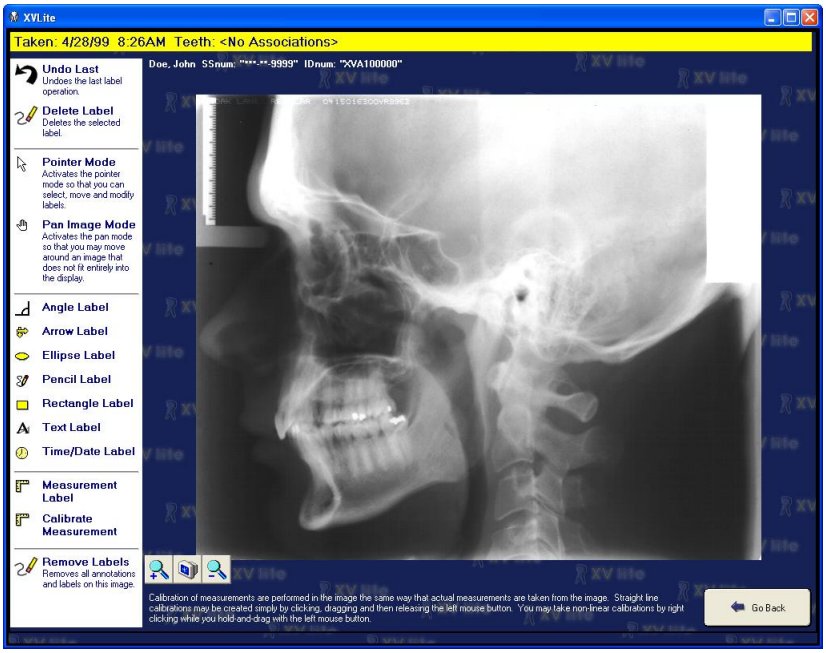
XVLite
Taken: 4/28/99 8:26AM Teeth: <No Associations>
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Undo Last
Undoes the last label operation.
Delete Label
Deletes the selected label.
Pointer Mode
Activates the pointer mode so that you can select, move and modify labels.
Pan Image Mode
Activates the pan mode so that you may move around an image that does not fit entirely into the display.
Angle Label
Arrow Label
Ellipse Label
Pencil Label
Rectangle Label
Text Label
Time/Date Label
Measurement Label
Calibrate Measurement
Remove Labels
Removes all annotations and labels on this image.
Calibration of measurements are performed in the image the same way that actual measurements are taken from the image. Straight line calibrations may be created simply by clicking, dragging and then releasing the left mouse button. You may take non-linear calibrations by right clicking while you hold-and-drag with the left mouse button.
Go Back

7.3.2.2 Select ***Labels*** from the menu bar to access the labeling options.

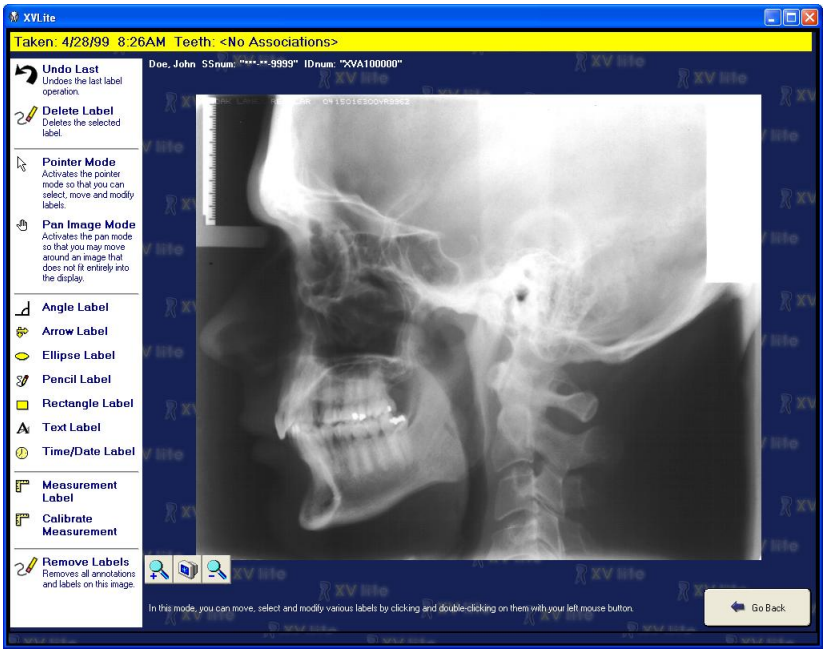
XVLite
Taken: 4/28/99 8:26AM Teeth: <No Associations>
Undo Last
Undoes the last label operation.
Delete Label
Deletes the selected label.
Pointer Mode
Activates the pointer mode so that you can select, move and modify labels.
Pan Image Mode
Activates the pan mode so that you may move around an image that does not fit entirely into the display.
Angle Label
Arrow Label
Ellipse Label
Pencil Label
Rectangle Label
Text Label
Time/Date Label
Measurement Label
Calibrate Measurement
Remove Labels
Removes all annotations and labels on this image.
In this mode, you can move, select and modify various labels by clicking and double-clicking on them with your left mouse button.
Go Back

7.3.2.3 Select ***Calibrate Measurement*** from the menu bar. The cursor will change into a crosshair with a gear above it.

7.3.2.4 Place the calibration crosshair at the starting point of the object of known length; single-click on the left mouse button; move the cross-hair to the end-point of the object; and then double-click on the left mouse button.

Non-linear calibrations can be created by left-clicking on mid-points while moving the mouse from point to point. Double-click on the left mouse button at the final end-point.

7.3.2.5 A 'Calibrate Measurements' pop-up screen will appear. Type in the correct length of the object. Click **OK**.

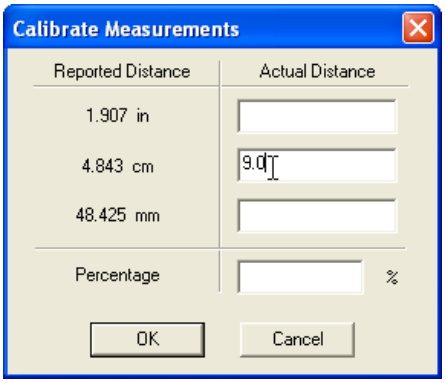

7.3.2.6 This image is now calibrated and any measurement performed will be based off the calibration.

7.3.3 Adding a Measurement Label

Follow the steps below to perform a measurement and create a measurement label.

7.3.3.1 Once a calibration is applied, the cursor changes to a crosshair with no gear, ready to take a measurement.

7.3.3.2 Place measurement crosshair at the starting point of the object to be measured; single-click on the left mouse button; move the cross-hair to the end-point of the object; and then double-click on the left mouse button.



Non-linear measurements can be created by right-clicking on end-points while dragging the mouse with the left button held down. Release the left mouse button at the final end-point.

7.3.3.3 A measurement label will be placed on the image displaying the measurement. Double-click on the measurement label to access the 'Measurement Properties' dialog box.

7.3.3.4 The 'Measurement' Properties dialog box displays to allow users to format the label. Customize the measurement label properties (color, line, unit, measurement position, etc.) then click **OK** to exit.

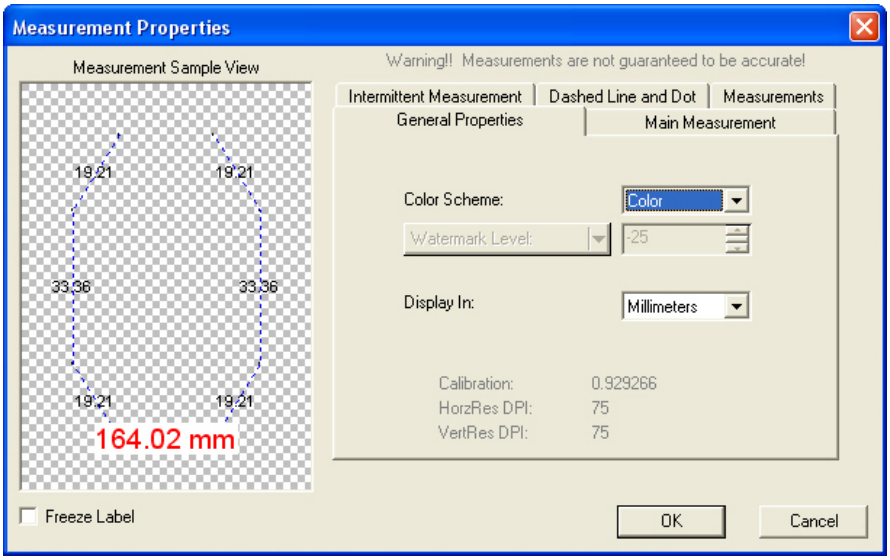

The 'Measurement Sample View' section in the dialog box above does not display the actual measurement, but rather a sample of what the measurement will look like. The 'Measurements'' tab is where to find the actual measurement.

7.3.3.5 To remove the measurement label, if desired, click on the label and then select **Delete Label**.

7.3.3.6 To add additional measurement labels to the calibrated image, select **Measurement Label** from the menu bar and repeat Steps 7.3.3.2 – 7.3.3.4.

7.3.3.7 When done, click on the **Go Back** button to return to the full view of the image. Since labels have been added to the image, the user will be prompted to save the changes. Click **Yes** to save the modification.

8 DISTRIBUTING IMAGES – TRANSIT™ ADD-ON COMPONENTS

8.1 General Information

The imaging application allows the addition of TransIT™ Communication Extension Devices (TransIT CEDs), additional components that expand the software's capabilities to include the sending of patient images, claim forms, etc. to referral doctors, insurance companies, etc. The commonly used TransIT CEDs are described in the following sections.

8.2 TransIT™ General Emailer Creator

8.2.1 Overview

The most commonly used TransIT™ add-on component, the General Emailer enables users to spawn their email client application (e.g. Microsoft® Outlook) and automatically attach patient images and files to a new email message. The General Emailer requires Outlook/Outlook Express or other MAPI clients.

8.2.2 Configuring the TransIT™ General Emailer Creator

The TransIT™ General Emailer component will attempt to use the default email application set up in Windows. Refer to Microsoft Support's Online Knowledgebase Article KB 154359 for instructions to specify Microsoft® Outlook or Outlook Express as the default email application.

8.2.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then Select ***Send*** on the menu bar.

8.2.2.2 The 'Select TransIT Method' dialog box appears. Click on **Access TransIT Options**.

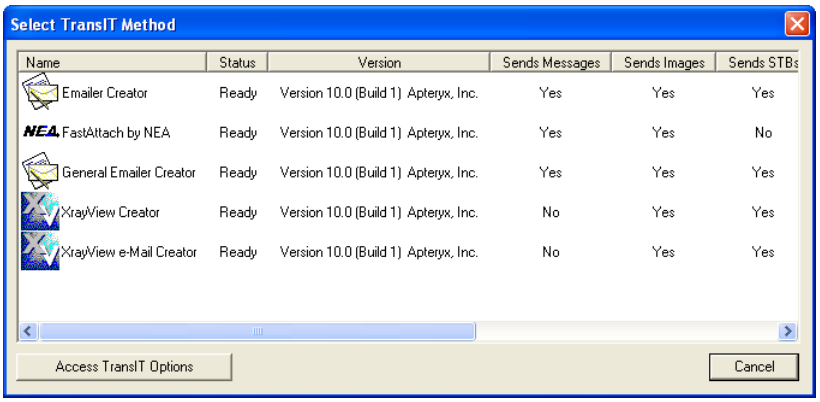

8.2.2.3 The 'TransIT Configurations' dialog box displays. Select General Emailer Creator and click on Edit Options.

8.2.2.4 The 'General Emailer Options' dialog box displays.

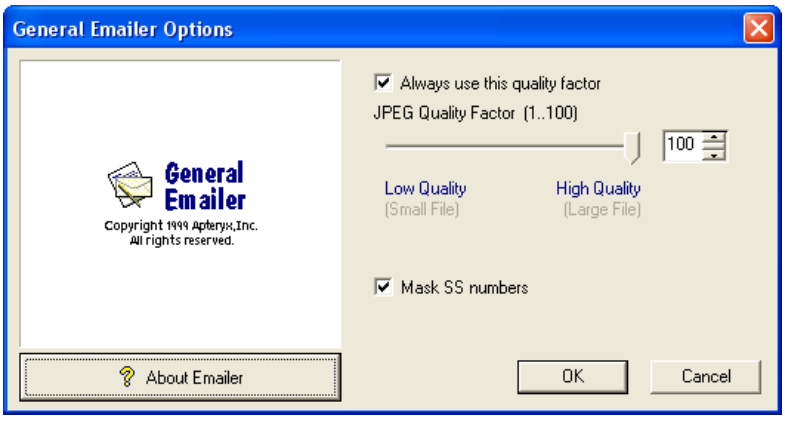

- Accept the default or change the 'JPEG Quality Factor' to whatever desired. The higher the quality the larger the generated jpeg files will be when converted and sent.
- Enable the **Mask SS numbers** option to suppress the transmission of SS numbers.
- Click **OK** when done.

8.2.2.5 Click OK on the 'TransIT Configurations' dialog to return to the 'Select TransIT Method' dialog box.

8.2.3 Sending Images Using the TransIT™ General Emailer Creator

8.2.3.1 On the 'Select TransIT Method' dialog box, select General Email Creator. The 'TransIT Item Selection' dialog box displays.

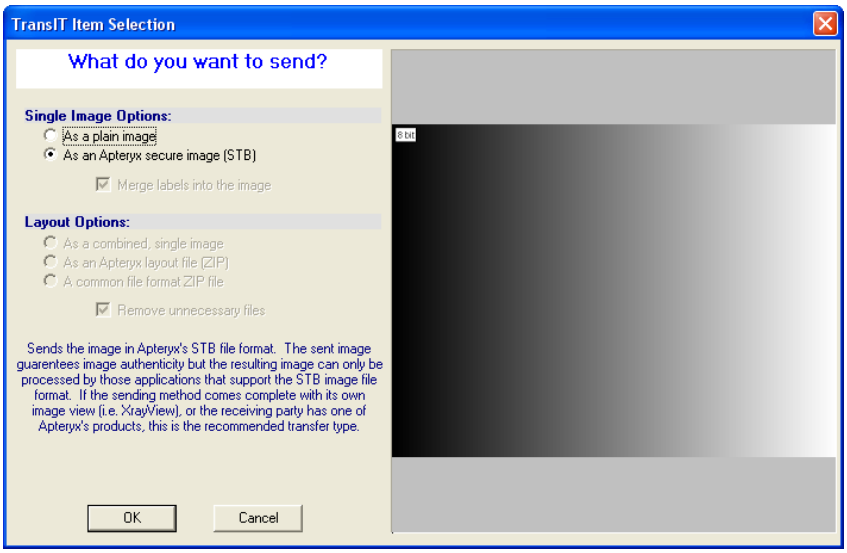
TransIT Item Selection
What do you want to send?
Single Image Options:
As a plain image
As an Apteryx secure image (STB)
Merge labels into the image
Layout Options:
As a combined, single image
As an Apteryx layout file (ZIP)
A common file format ZIP file
Remove unnecessary files
Sends the image in Apteryx's STB file format. The sent image guarentees image authenticity but the resulting image can only be processed by those applications that support the STB image file format. If the sending method comes complete with its own image view (i.e. XrayView), or the receiving party has one of Apteryx's products, this is the recommended transfer type.
OK
Cancel

- 'Single Image Options': If sending one or more single images, specify whether to send them as a plain image (i.e. JPEG format) or as an STB files the 'Single Image Options' section.
- Layout Options: If sending one or more layouts, select one of the following file format options:
  - **As a combined, single image** (i.e. JPEG format)
  - **As an Apteryx layout file** (i.e. a compressed zip file containing the layout, STB images, and related data files
  - **A common file format ZIP file** (i.e. a compressed zip file containing the images in JPEG format).

8.2.3.2 Click on **OK**. The 'TransIT Emailer Information' screen displays. Complete the following information on each tab:

- 'General' tab: Complete the 'Subject' and 'Reference Number' fields.

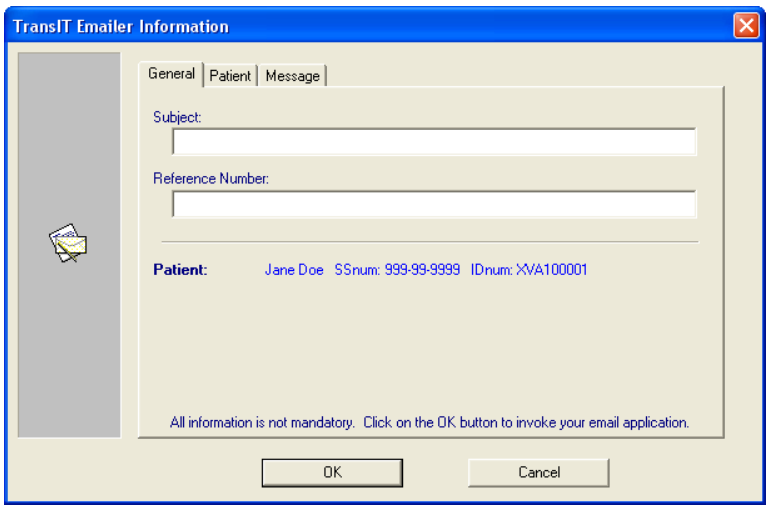

- 'Patient' tab: The tab is pre-populated with the open patient's information. Complete any required field if blank.

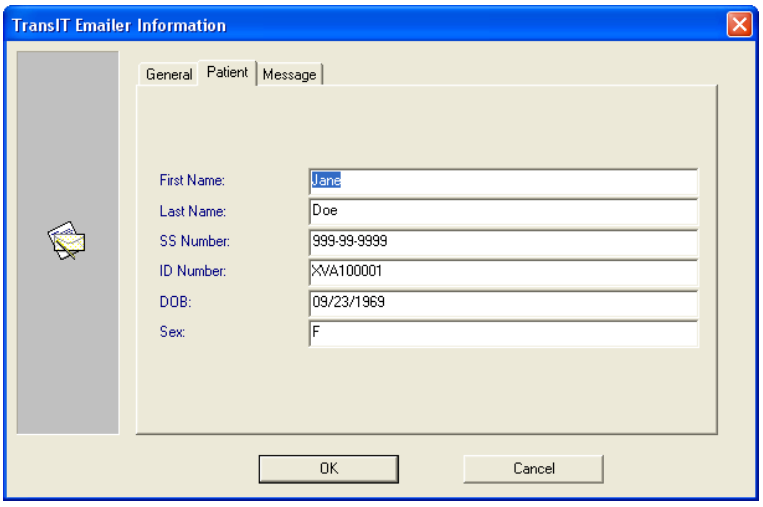

- ‘Message’ tab: Enter a message for the recipient of the email. The message entered will appear in the body of the email.

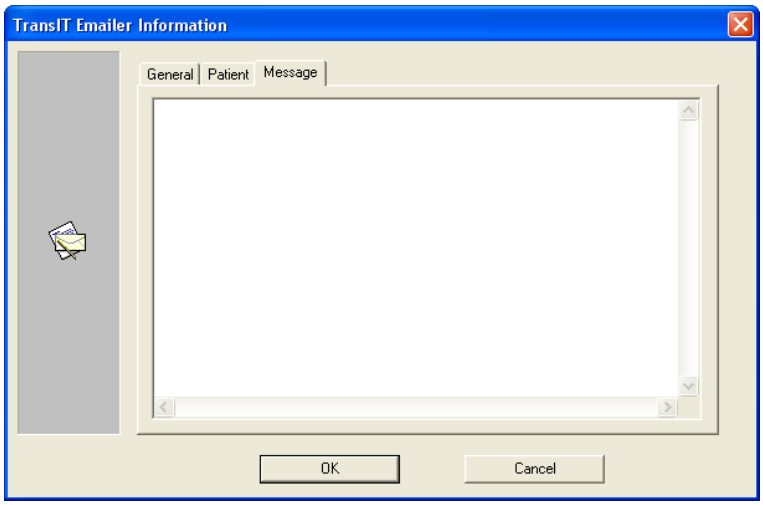

8.2.3.3 Click **OK** when the ‘TransIT Emailer Information’ tabs have been completed. The imaging application proceeds to spawn Outlook/Outlook Express create new email is created with the image attached.

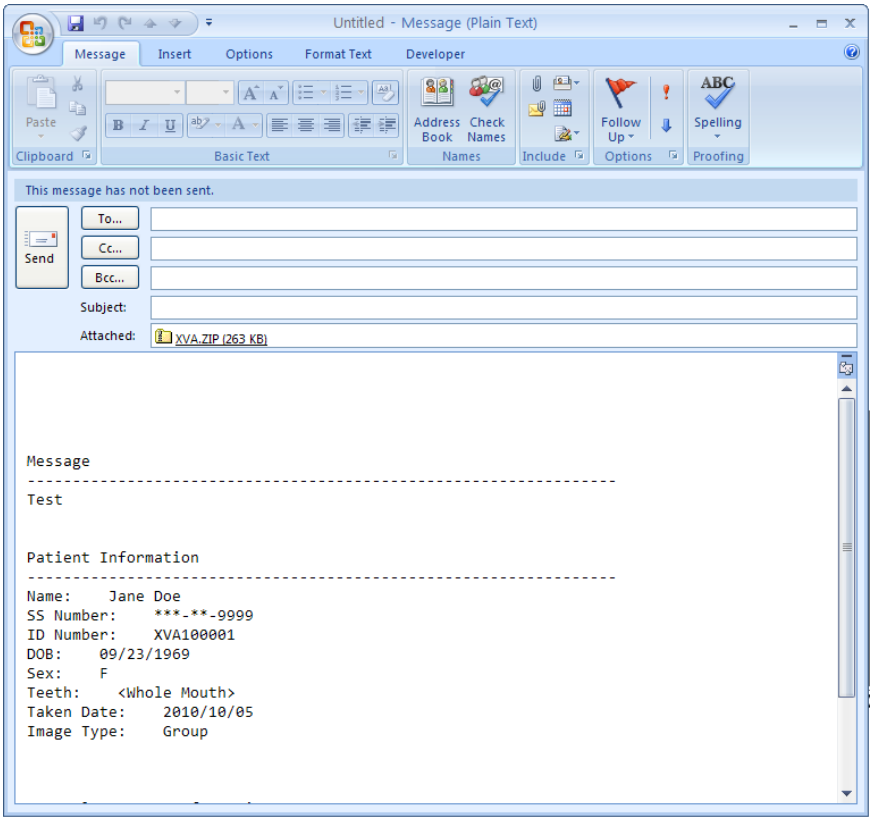

8.2.3.4 Add the email information of the recipient and proceed to send the attached image/layout in Outlook/Outlook Express.

8.3 TransIT™ Emailer Creator

8.3.1 Overview

The Emailer Creator module enables the sending of emails from within the imaging application. Multiple patient images and files can be sent directly through a dental

practice's Internet Service Provider (ISP). Outlook/Outlook Express is not required with this extension.

8.3.2 Configuring Emailer Options:

For the TransIT™ Emailer component to function an outgoing SMTP mail server must be configured. The Emailer is only compatible with outgoing mail servers that DO NOT require authentication or encryption (e.g. SSL) for transmission. Contact your ISP for outgoing SMTP server information and transmission requirements.

8.3.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select Send on the menu bar.

8.3.2.2 The 'Select TransIT Method' dialog box appears. Click on **Access TransIT Options**.

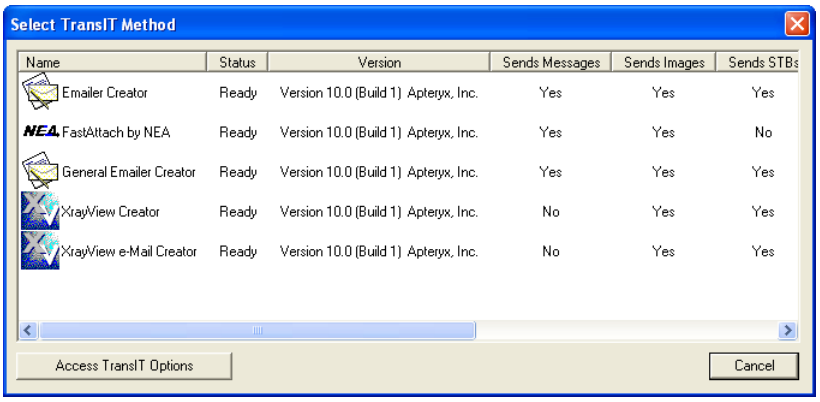

8.3.2.3 The 'TransIT Configurations' dialog box displays. Select **Emailer Creator** and click on **Edit Options**.

8.3.2.4 The 'General Emailer Options' dialog box displays.

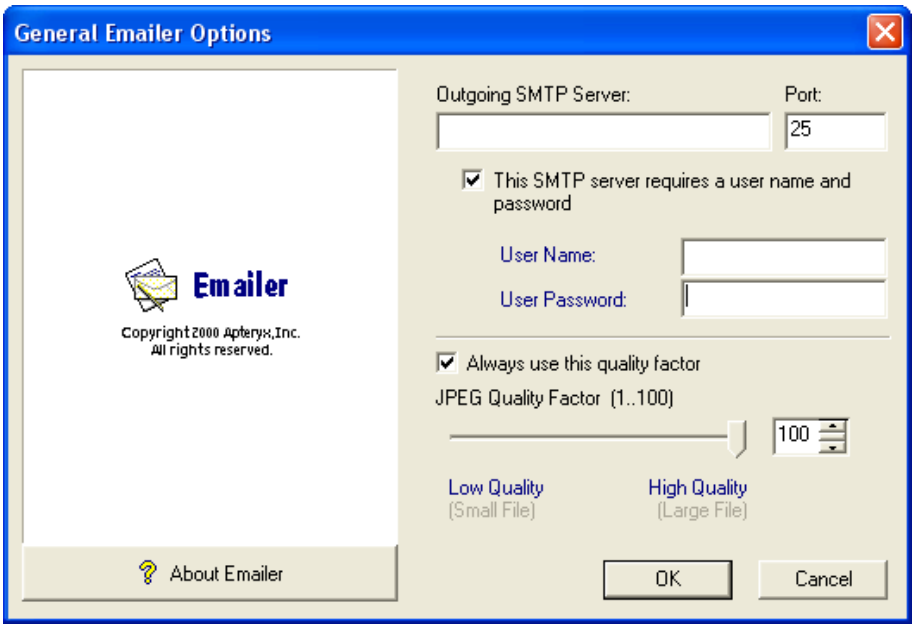

- Complete the 'Outgoing SMTP Server' and 'Port' fields.
- Click to enable the option **This SMTP server requires a user name and password**. Complete the 'User Name' and 'User Password' fields.
- Accept the default or change the 'JPEG Quality Factor' to whatever desired. The higher the quality the larger the generated jpeg files will be when converted and sent.
- Click **OK** when done.

8.3.2.5 Click OK on the 'TransIT Configurations' dialog to return to the 'Select TransIT Method' dialog box.

8.3.3 Sending Images Using the TransIT™ Emailer Creator:

8.3.3.1 On the 'Select TransIT Method' dialog box, select Email Creator. The 'TransIT Item Selection' dialog box displays.

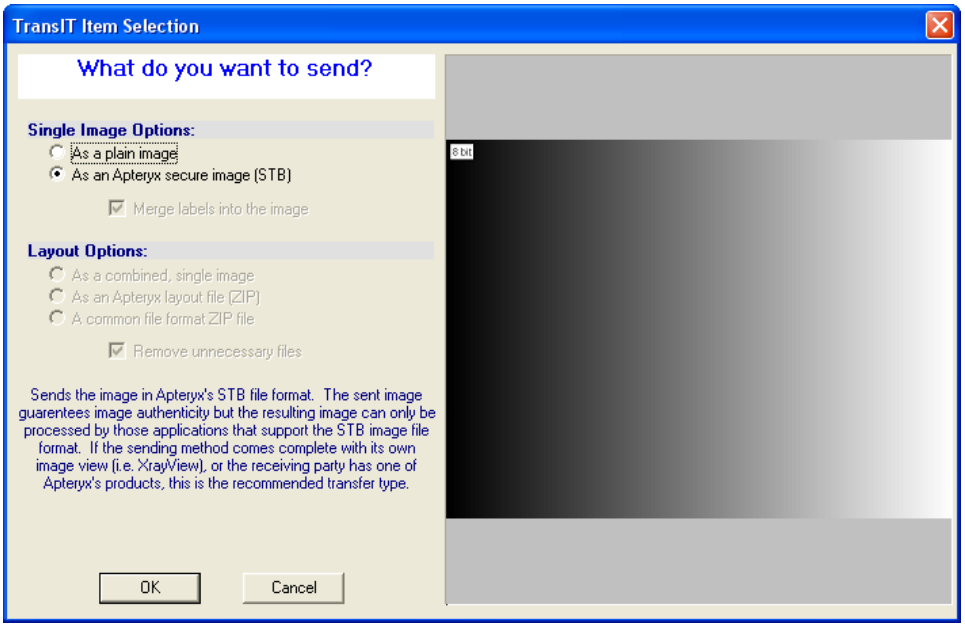
TransIT Item Selection
What do you want to send?
Single Image Options:
As a plain image
As an Apteryx secure image (STB)
Merge labels into the image
Layout Options:
As a combined, single image
As an Apteryx layout file (ZIP)
A common file format ZIP file
Remove unnecessary files
Sends the image in Apteryx's STB file format. The sent image guarentees image authenticity but the resulting image can only be processed by those applications that support the STB image file format. If the sending method comes complete with its own image view (i.e. XrayView), or the receiving party has one of Apteryx's products, this is the recommended transfer type.
OK
Cancel
8 bit

- 'Single Image Options': If sending one or more single images, specify whether to send them as a plain image (i.e. JPEG format) or as an STB files the 'Single Image Options' section.
- Layout Options: If sending one or more layouts, select one of the following file format options:
  - **Combined, single image** (i.e. JPEG format)
  - **Apteryx layout file** (i.e. a compressed zip file containing the layout, STB images, and related data files
  - **A common file format ZIP file** (i.e. a compressed zip file containing the images in JPEG format).

8.3.3.2 Click on **OK** to generate and send the email via the outgoing SMTP server.

8.4 FastAttach by NEA

8.4.1 Overview

The FastAttach module enables users to submit patient images and claims to NEA's FastAttach web-based service.

8.4.2 Configuring FastAttach Options:

8.4.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select ***Send*** on the menu bar.

8.4.2.2 The 'Select TransIT Method' dialog box appears. Click on **Access TransIT Options**.

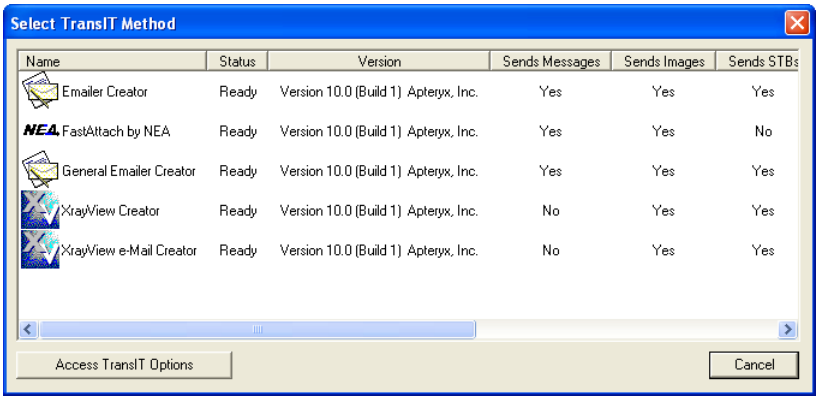

8.4.2.3 The 'TransIT Configurations' dialog box displays. Select **FastAttach by NEA** and click on **Edit Options**.

8.4.2.4 The 'FastAttach Options' dialog box displays.

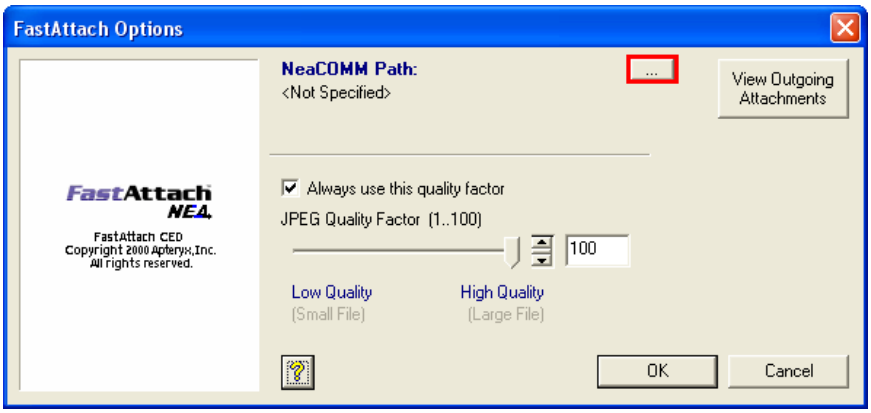

- Select the button shown in red above to find/specify the location of the NEACOMM application.
- Accept the default or change the 'JPEG Quality Factor' to whatever desired. The higher the quality the larger the generated jpeg files will be when converted and sent.
- Click **OK** when done.

8.4.2.5 Click **OK** on the 'TransIT Configurations' dialog to return to the 'Select TransIT Method' dialog box.

8.4.3 Submitting Patient Images/Claims Using FastAttach by NEA:

8.4.3.1 On the 'Select TransIT Method' dialog box, select **Fast Attach by NEA**. The 'TransIT Selection' dialog box displays. Click **OK** to continue.

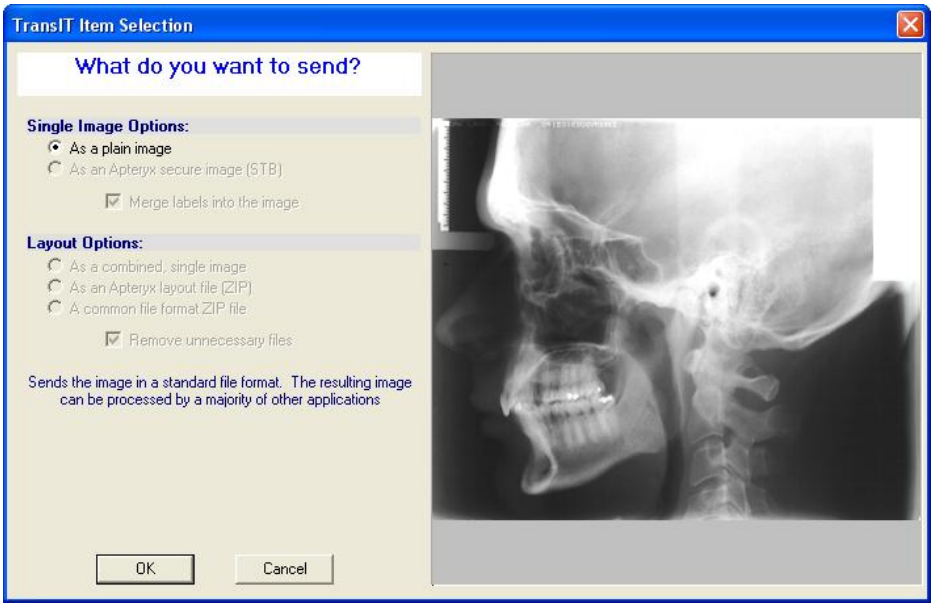
TransIT Item Selection
What do you want to send?
Single Image Options:
As a plain image
As an Apteryx secure image (STB)
Merge labels into the image
Layout Options:
As a combined, single image
As an Apteryx layout file (ZIP)
A common file format ZIP file
Remove unnecessary files
Sends the image in a standard file format. The resulting image can be processed by a majority of other applications
OK
Cancel

8.4.3.2 The 'TransIT Fast Attach Information' dialog box displays. Complete the following information on each tab:

- 'General' tab: Select the applicable date range of service using the calendars. Enter the optional 'Payor Reference Number' and 'Claim Amount.

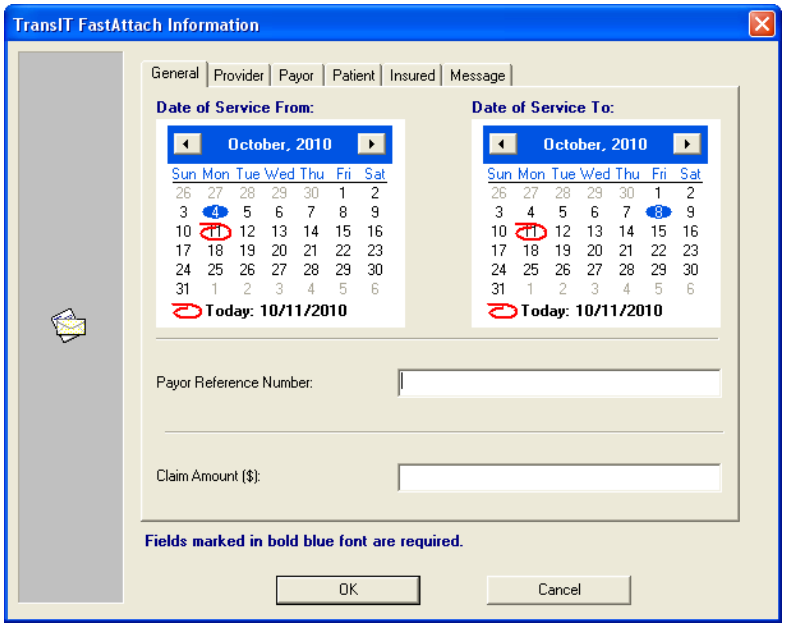

- 'Provider' tab: Enter the required dental practice information. Click the **Add** button to store the entered information as a quick entry for future use.

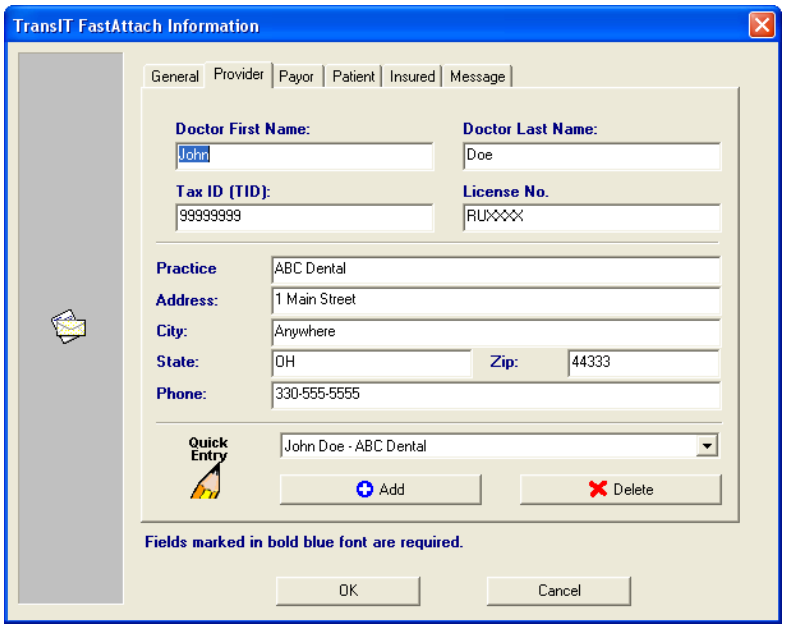

- 'Payor' tab: The 'Payor Name' is the insurance company the patient is insured through.

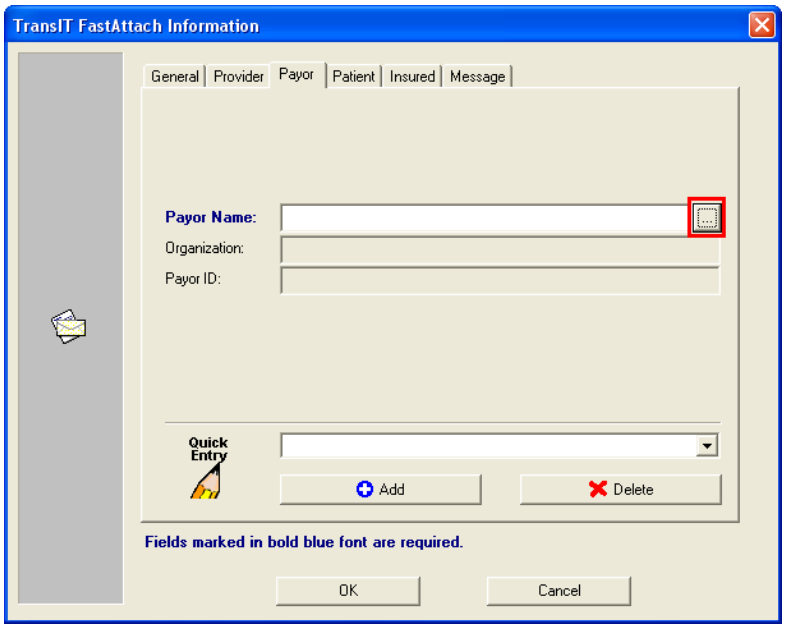

- Select the **Browse** button, shown in red above, to launch and select the patient's insurance company from the 'Select NEA Player' dialog box.

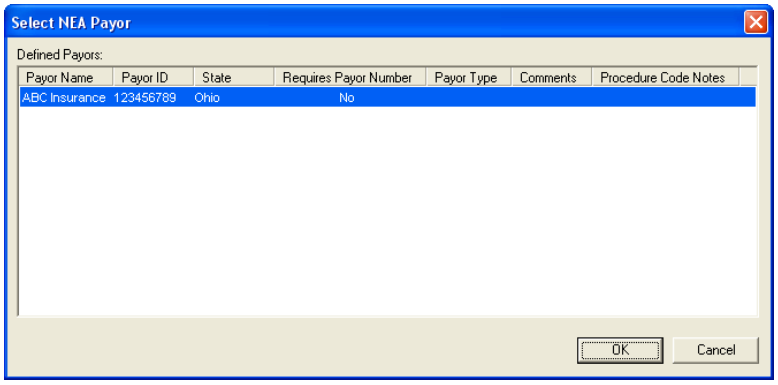

- Click **OK** to return to the 'Payor' tab.
- Click the **Add** button to store the entered information as a quick entry for future use.

- 'Patient' tab: The tab is pre-populated with the open patient's information. Complete any required field if blank.

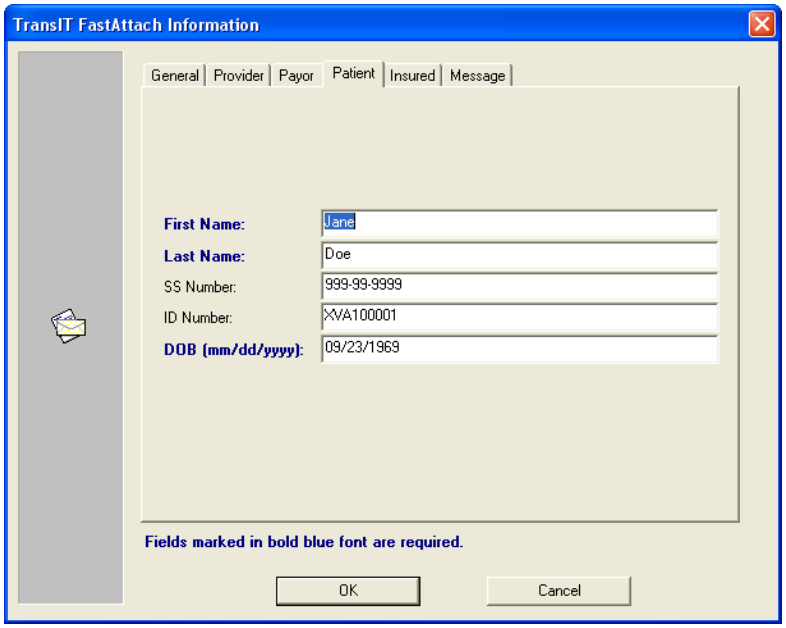

- 'Insured' tab: If the patient is not the insured person (e.g. a dependant or spouse), enter the insured person's information and select the applicable relationship. If the patient is the insured person, select the **Same as patient** button to auto-populate the fields.

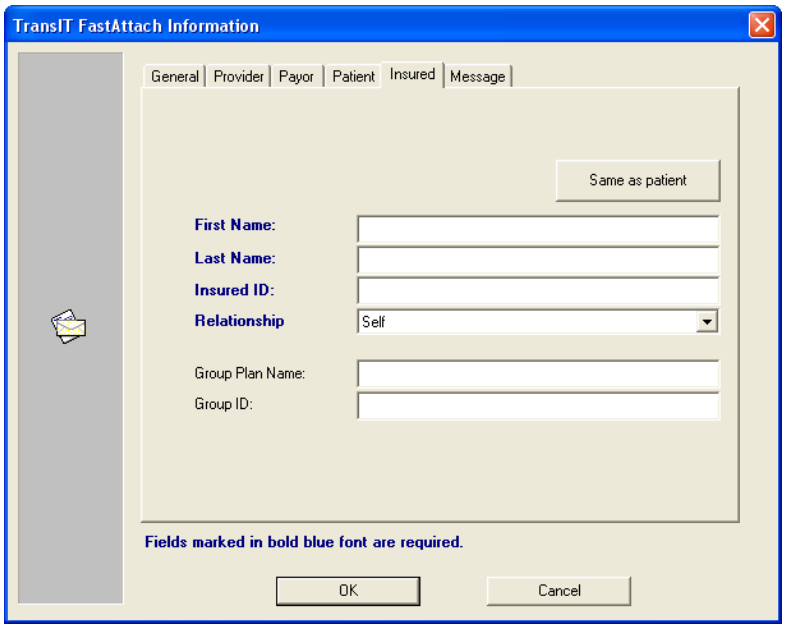

- 'Message' tab: Enter any additional information to relay to the Insurance Company regarding the claim and/or attachments.

8.4.3.3 Click **OK** to forward the image and claim information to NEA's FastAttach communication application.

8.5 XrayView™ e-Mailer Creator

8.5.1 Overview

The XrayView™ e-Mailer Creator creates a ZIP file or self-extracting executable (XrayViewMailer.zip or XrayView.exe) containing a patients images. The XrayView™ e-Mailer Creator then calls up a user's email client application (e.g. Microsoft® Outlook) and attaches the file in a new email message. Email recipients that receive the attachment can then detach, run the file, and view the provided images within an XrayView™ interface. XrayView™ e-Mailer Creator supports the transmission of Apteryx's unmodifiable, Secure Tagged Block (STB) file format, guaranteeing image authenticity.

8.5.2 Configuring the XrayView™ e-Mailer Creator Options

The XrayView™ e-Mailer component will attempt to use the default email application set up in Windows. Refer to Microsoft Support's Online Knowledgebase Article KB 154359 for instructions to specify Microsoft® Outlook or Outlook Express as the default email application.

8.5.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select ***Send*** on the menu bar.

8.5.2.2 The 'Select TransIT Method' dialog box appears. Click on **Access TransIT Options**.

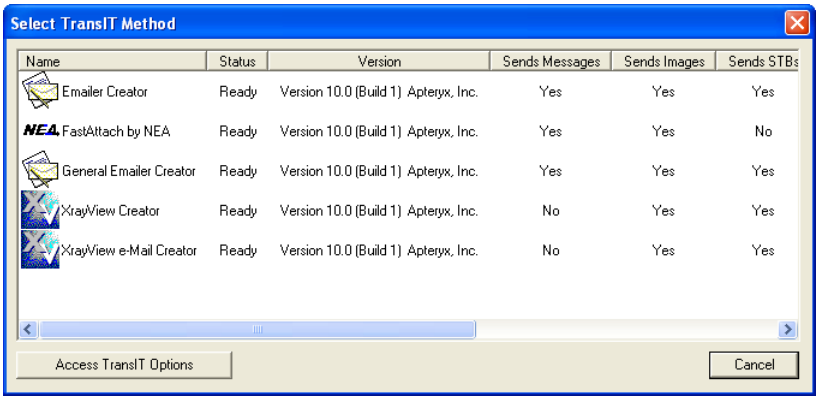

8.5.2.3 The 'TransIT Configurations' dialog box displays. Select **XrayView e-Mail Creator** and click on **Edit Options**.

8.5.2.4 The 'XrayView e-Mailer Options' dialog box displays.

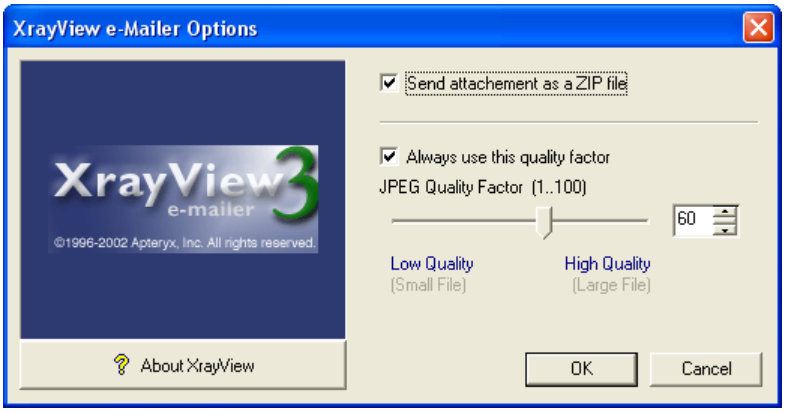

- Enable Send attachment as a ZIP file to generate attachments as a ZIP file. If disabled, the attachment will attach a self-extracting executable (*.EXE file extension).

  ⚠ **Warning:** Some email clients may be configured not to accept *EXE file extensions for security reasons. If so, the email client will strip out the attachment when the new message is sent.

- Accept the default or change the 'JPEG Quality Factor' to whatever desired. The higher the quality the larger the generated jpeg files will be when converted and sent.
- Click **OK** when done.

8.5.2.5 Click **OK** on the 'TransIT Configurations' dialog to return to the 'Select TransIT Method' dialog box'.

8.5.3 Sending Images Using the XrayView e-Mailer Creator

8.5.3.1 On the 'Select TransIT Method' dialog box, select **XrayView e-Mail Creator**. The 'TransIT Item Selection' dialog box displays.

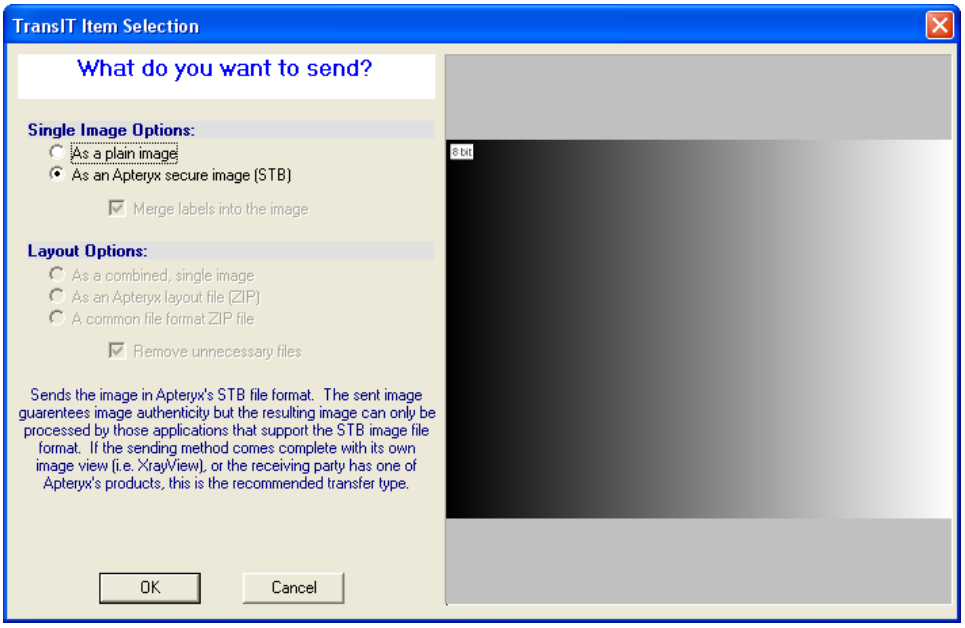
TransIT Item Selection
What do you want to send?
Single Image Options:
As a plain image
As an Apteryx secure image (STB)
Merge labels into the image
Layout Options:
As a combined, single image
As an Apteryx layout file (ZIP)
A common file format ZIP file
Remove unnecessary files
Sends the image in Apteryx's STB file format. The sent image guarentees image authenticity but the resulting image can only be processed by those applications that support the STB image file format. If the sending method comes complete with its own image view (i.e. XrayView), or the receiving party has one of Apteryx's products, this is the recommended transfer type.
OK
Cancel

- 'Single Image Options': If sending one or more single images, specify whether to send them as a plain image (i.e. JPEG format) or as an STB files the 'Single Image Options' section.
- 'Layout Options': If sending one or more layouts, select one of the following file format options:
  - **Combined, single image** (i.e. JPEG format)
  - **Apteryx layout file** (i.e. a compressed zip file containing the layout, STB images, and related data files
  - **A common file format ZIP file** (i.e. a compressed zip file containing the images in JPEG format).

8.5.3.2 Click **OK**. The 'TransIT XrayView Information' screen displays. Complete the following information on each tab:

- 'General' tab: Complete the 'Subject' and 'Reference Number' fields.

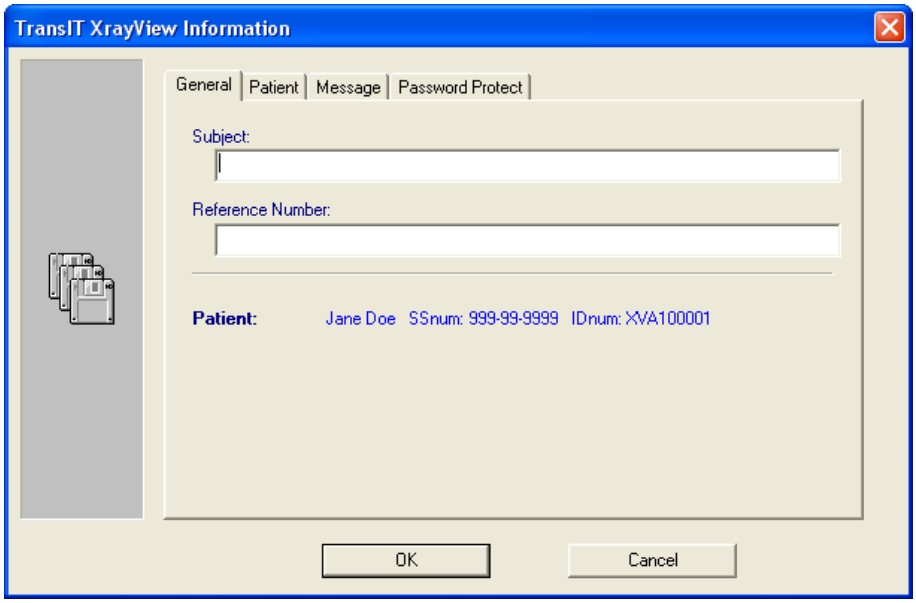

- 'Patient' tab: The tab is pre-populated with the open patient's information. Complete any required field if blank.

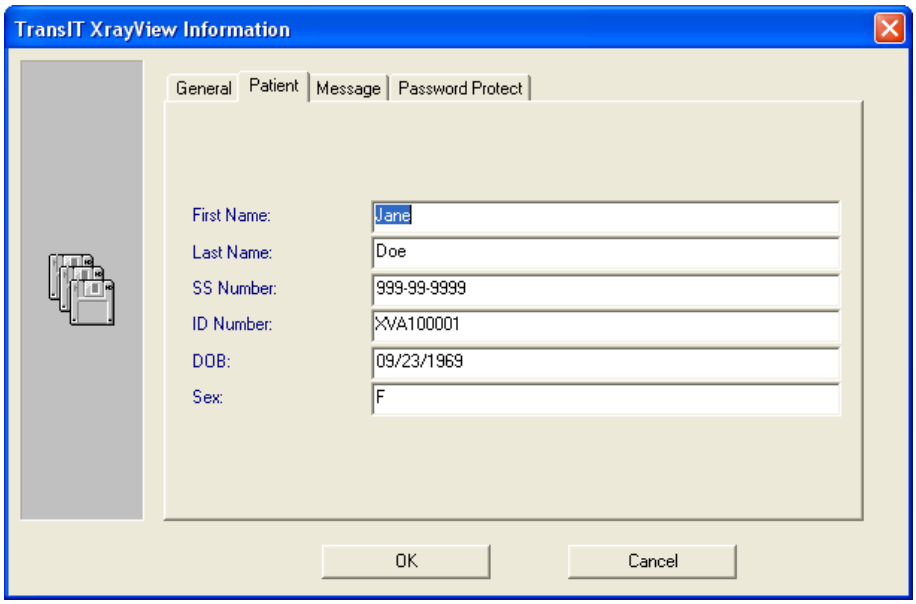

- 'Message' tab: Enter information for the recipient of the email.

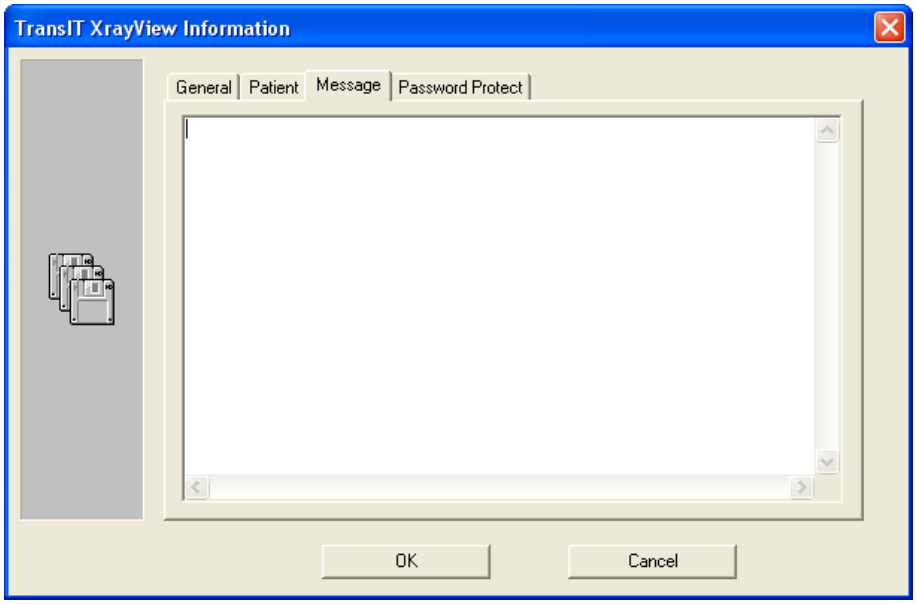

- 'Password Protect' tab: If desired, enable the **Password protect the image** option and enter a password in the 'Password' field. The recipient will need to be provided the password in order to access the files in the attachment when sent.

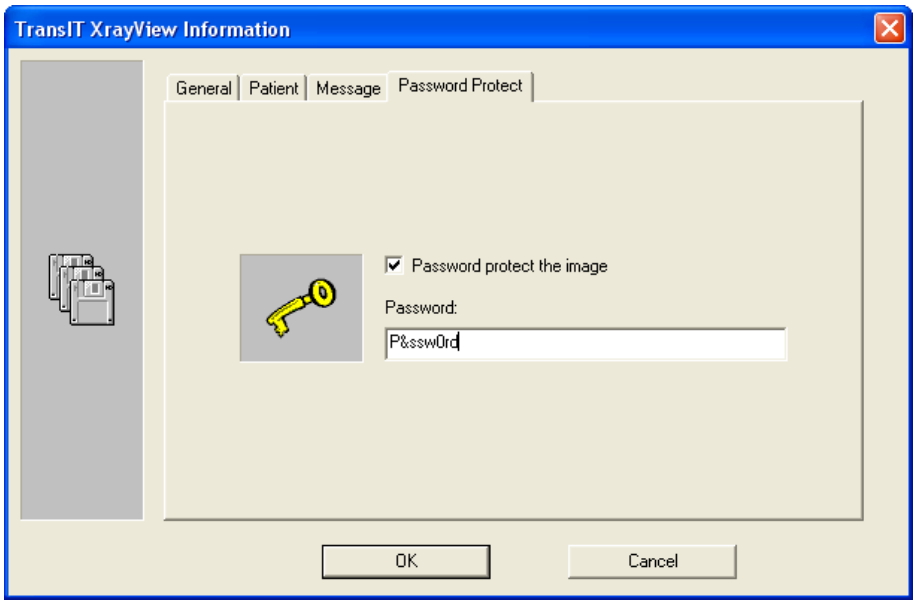

8.5.3.3 Click **OK** when the 'TransIT XrayView Information' tabs have been completed. The imaging application proceeds to spawn Outlook/Outlook Express create new email is created with the image attached.

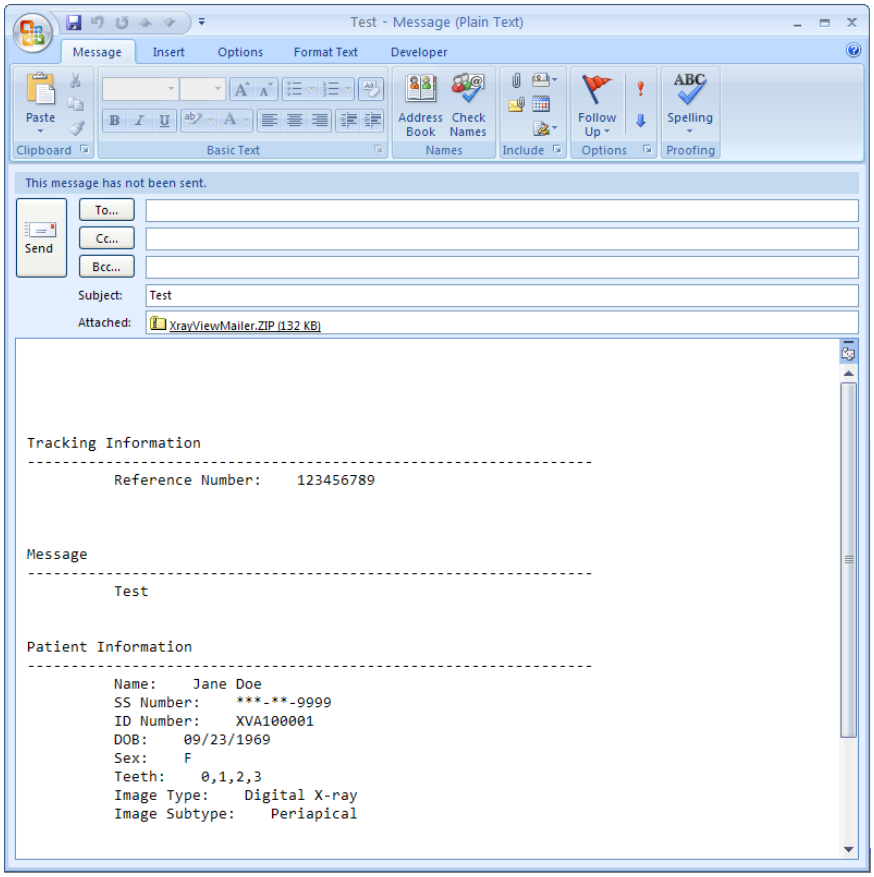

8.5.3.4 Add the recipient's email information and proceed to send the attached image/layout in Outlook/Outlook Express.

8.6 XrayView™ Creator

8.6.1 Overview

The XrayView Creator creates a self-extracting executable (XrayView.exe) containing a patients images and information that can be saved on various removable media (e.g. USB flash drive, external hard disk, etc.) and provided to other dentist/practices for referrals, etc. Recipients that are provided the file can then run the file and view the provided images within an XrayView™ interface. XrayView™ Creator supports the transmission of Apteryx's unmodifiable, Secure Tagged Block (STB) file format, guaranteeing image authenticity.

8.6.2 Configuring the XrayView™ Creator Options

8.6.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select Send on the menu bar.

8.6.2.2 The 'Select TransIT Method' dialog box appears. Click on **Access TransIT Options**.

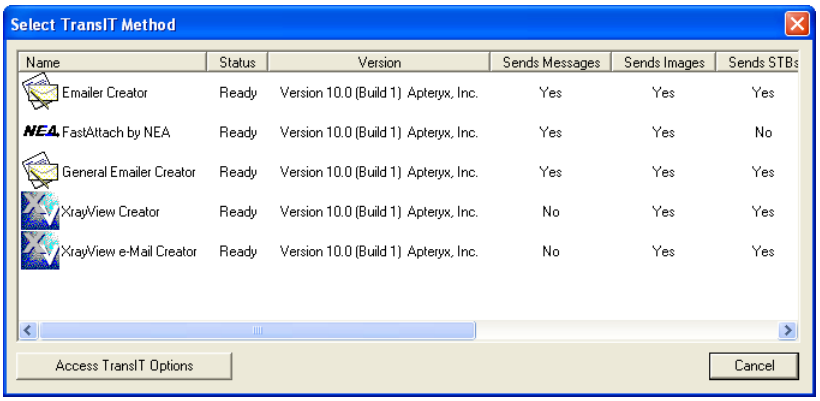

8.6.2.3 The 'TransIT Configurations' dialog box displays. Select **XrayView Creator** and click on **Edit Options**.

8.6.2.4 The 'XrayView Options' dialog box displays.

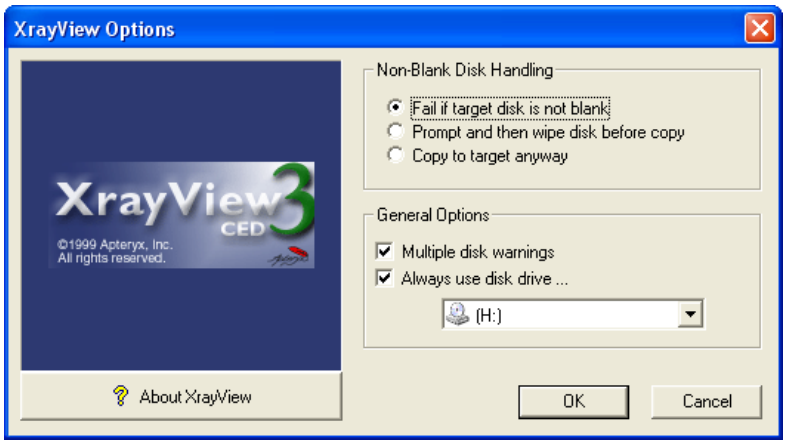

- Enable an applicable option in the 'Non-blank Disk Handling' section:
  - **Fail if target disk is not blank** – If enabled, the XrayView.exe file will not be created in the specified destination unless the destination is blank. This option is useful if the destination contains XrayView files that a user may not want to overwrite. The user can only write to the destination if the media is blank.

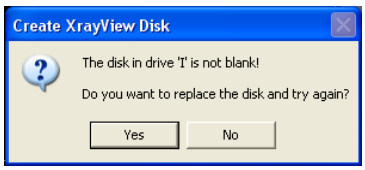

- **Prompt and then wipe disk before copy** – If enabled, the user will be prompted with a warning that the destination will be erased before the XrayView.exe file is created. This option is useful if the destination location has limited disk space.

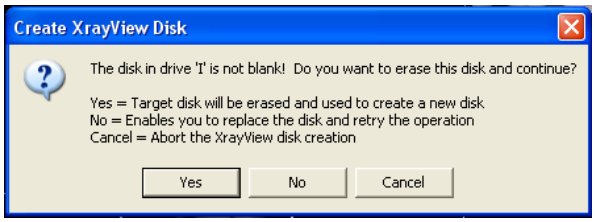
Create XrayView Disk
The disk in drive 'I' is not blank! Do you want to erase this disk and continue?
Yes = Target disk will be erased and used to create a new disk
No = Enables you to replace the disk and retry the operation
Cancel = Abort the XrayView disk creation
Yes
No
Cancel

- **Copy to target anyway** – If selected, any pre-existing XrayView files will be overwritten without warning.

- Accept the default or change the 'JPEG Quality Factor' to whatever desired. The higher the quality the larger the generated jpeg files will be when converted and sent.
- Click **OK** when done.

8.6.2.5 Click **OK** on the 'TransIT Configurations' dialog to return to the 'Select TransIT Method' dialog box.

8.6.3 Distributing Images Using the XrayView Creator

8.6.3.1 On the 'Select TransIT Method' dialog box, select XrayView Creator. The 'TransIT Item Selection' dialog box displays.

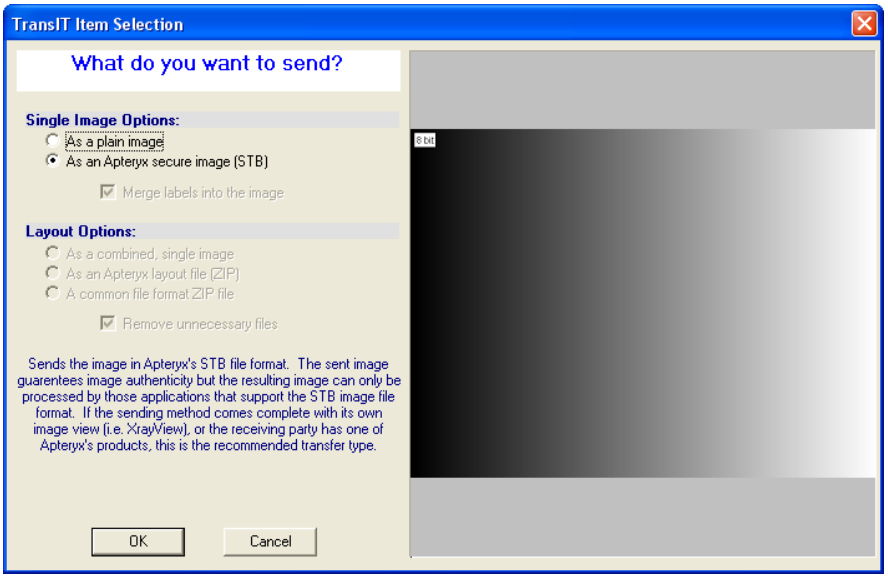
TransIT Item Selection
What do you want to send?
Single Image Options:
As a plain image
As an Apteryx secure image (STB)
Merge labels into the image
Layout Options:
As a combined, single image
As an Apteryx layout file (ZIP)
A common file format ZIP file
Remove unnecessary files
Sends the image in Apteryx's STB file format. The sent image guarentees image authenticity but the resulting image can only be processed by those applications that support the STB image file format. If the sending method comes complete with its own image view (i.e. XrayView), or the receiving party has one of Apteryx's products, this is the recommended transfer type.
OK
Cancel

- 'Single Image Options': If sending one or more single images, specify whether to send them as a plain image (i.e. JPEG format) or as an STB files the 'Single Image Options' section.
- Layout Options: If sending one or more layouts, select one of the following file format options:
  - **Combined, single image** (i.e. JPEG format)
  - **Apteryx layout file** (i.e. a compressed zip file containing the layout, STB images, and related data files
  - **A common file format ZIP file** (i.e. a compressed zip file containing the images in JPEG format).

8.6.3.2 Click **OK**. The 'TransIT XrayView Information' screen displays. Complete the following information on each tab:

- 'General' tab: Complete the 'Subject' and 'Reference Number' fields.

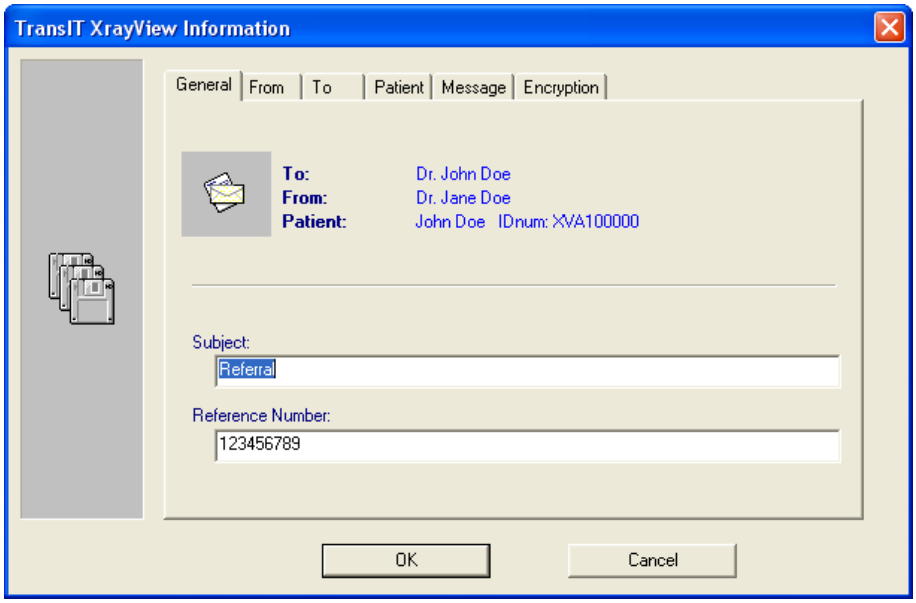

- 'From' tab: Enter the doctor and dental practice information. Select the **Add 'FROM' Entry** button to store the information as a quick entry for future use.

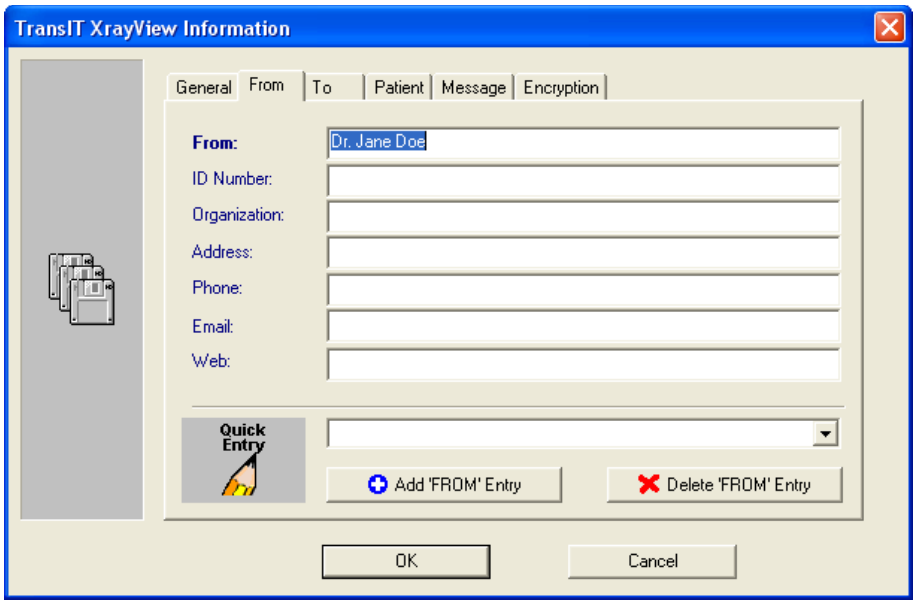

- 'To' tab: Enter the recipient's information. Select the **Add 'To' Entry** button to store the information as a Quick Entry for future use.

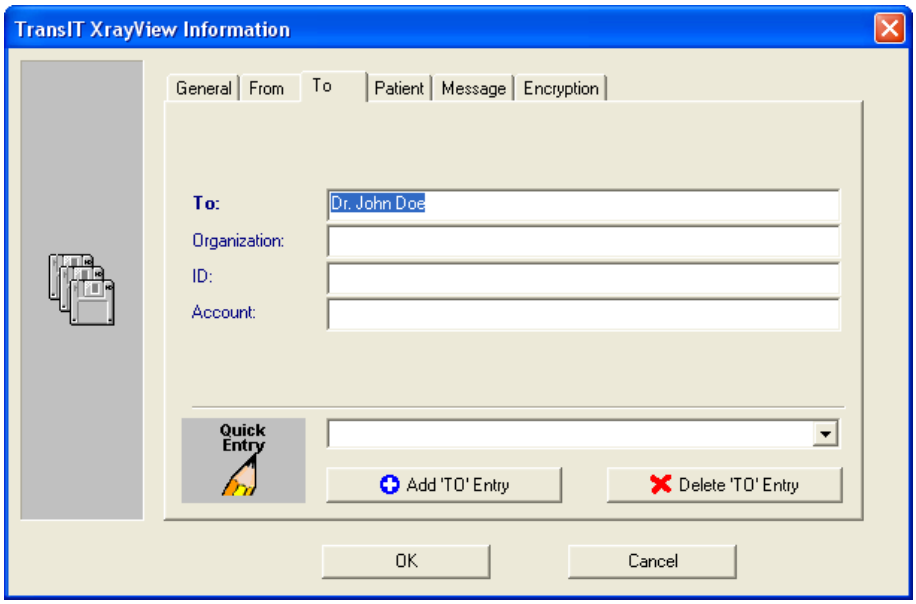

- 'Patient' tab: The tab is pre-populated with the open patient's information. Complete any required field if blank.

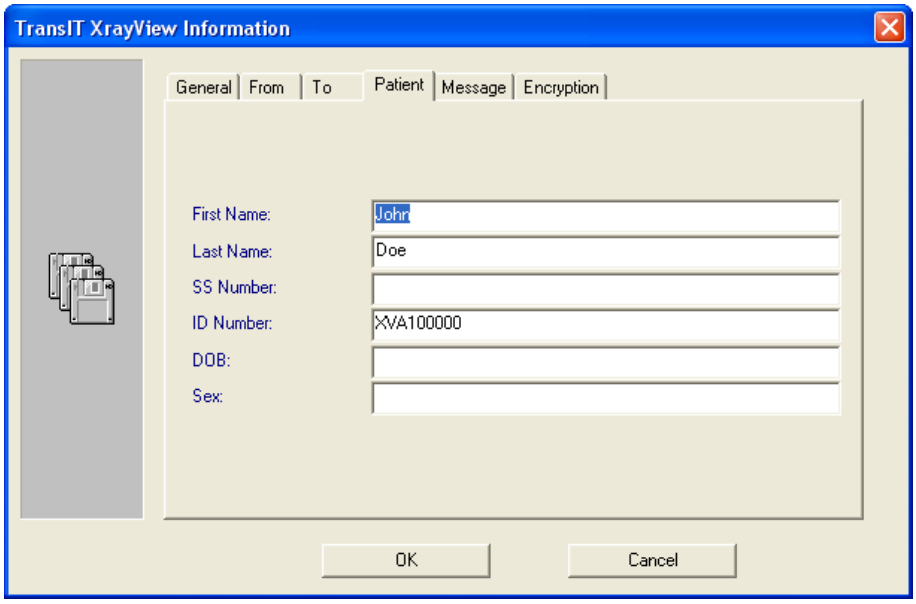

- ‘Message’ tab: Enter information for the recipient of the email.

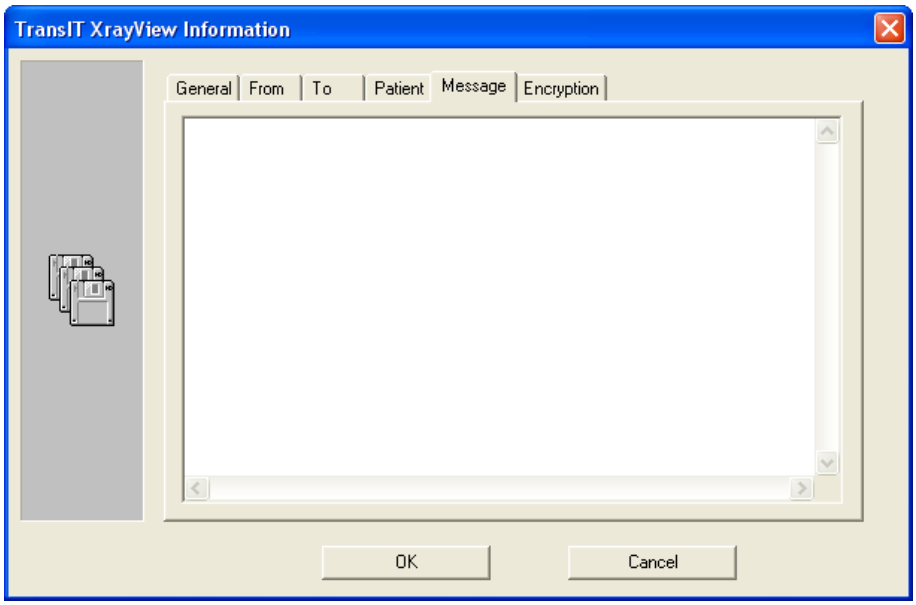

- ‘Encryption’ tab: If desired, enable the encryption option to encrypt the image and enter a password in the ‘Password’ field. The recipient will need to be provided the password in order to access the files in the attachment when sent.

8.6.3.3 Click **OK** when the ‘TransIT XrayView Information’ tabs have been completed.

8.6.3.4 Follow the prompts to generate the XrayView files in the destination specified.

9 PRINTING IMAGES AND IMAGE-RELATED DOCUMENTS

9.1 General Information

The imaging application has built in print functionality that allows users to print images and related information directly to a local or networked printer. In addition, users have access to a library of customizable Document Templates that can be used to generate referral letters, treatment plans, etc. in Microsoft® Word.

9.2 Printing a Single Image

9.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select Print on the menu bar.

9.2.2 The Wizard advances to the print utility.

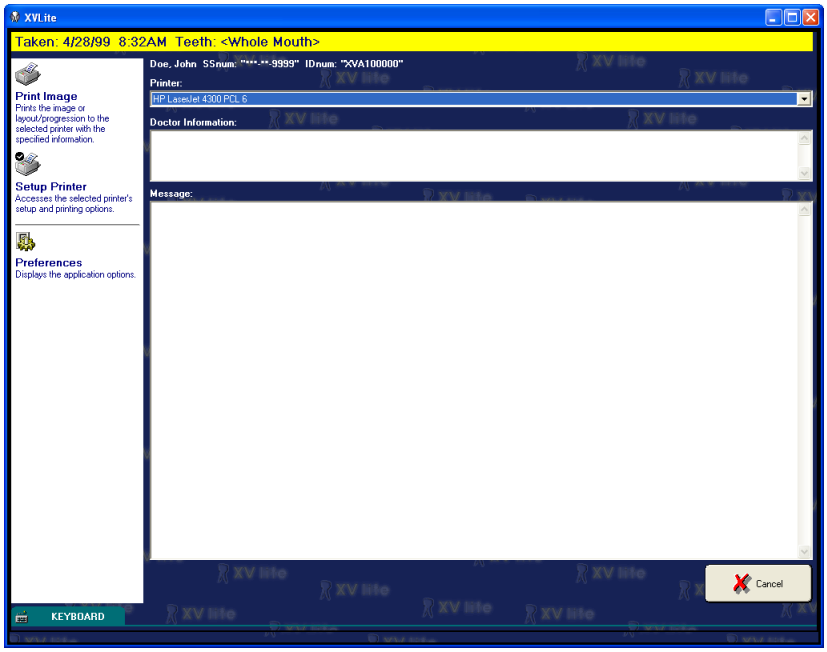

9.2.2.1 Select the desired printer off the 'Printer' drop-down list.

9.2.2.2 Complete the 'Doctor's Information' text box, if desired, that should be printed with the image.

9.2.2.3 Complete the 'Message' text, if desired.

9.2.3 Select **Print Image** off the menu bar to print the image to the select printer.

9.3 Printing Multiple Images

9.3.1 View an existing patient's images and then select **Print Multiple Images** off the menu bar.

9.3.2 The Wizard will advance to an image selection screen.

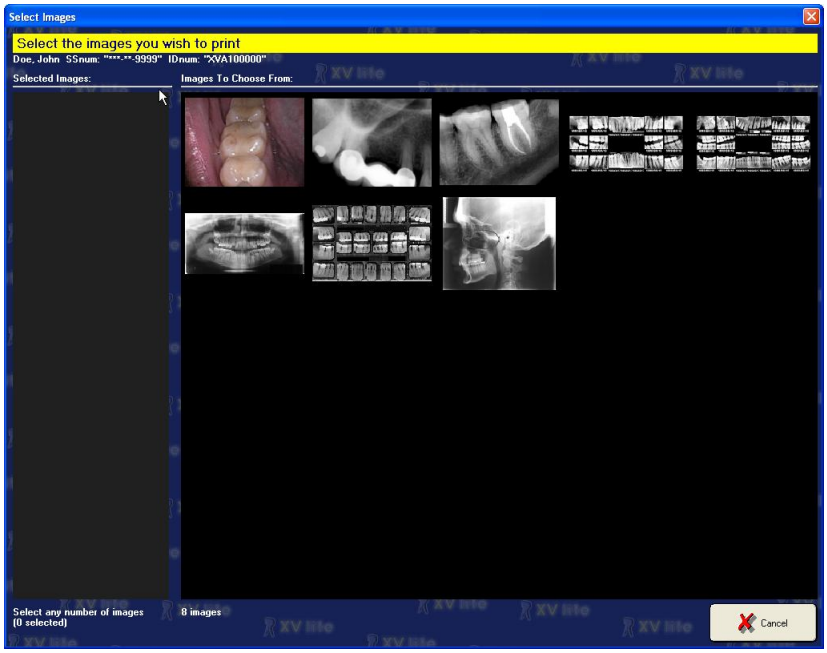

9.3.2.1 The 'Images To Chose From' section on the right displays the current images in the patient's record. Click on each desired image to add to the print job.

9.3.2.2 Each image that is added to the print job will display in the 'Selected Images' section on the left. If the wrong image is selected, click on it once to remove it.

9.3.2.3 When ready to proceed with the print job, click on **OK**.

9.3.3 The Wizard advances to the multiple image print utility.

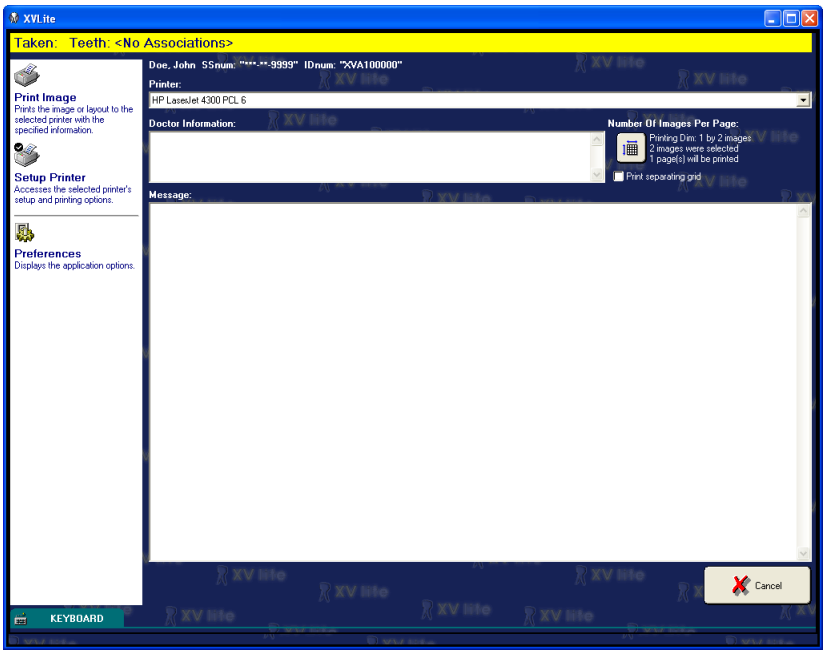

9.3.3.1 Select the desired printer off the 'Printer' drop-down list.

9.3.3.2 Complete the 'Doctor's Information' text box, if desired, that should be printed with the image.

9.3.3.3 To the right, the 'Number of Images Per Page' section indicates the way the images will be printed on a grid and the total number of pages.

9.3.3.4 Click on the button to reconfigure the layout of the print job. Use the mouse to select the desired number of columns and rows for the image grid.

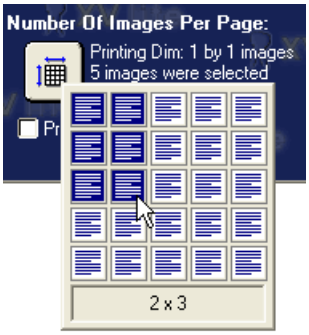

9.3.3.5 Complete the 'Message' text, if desired.

9.3.4 Select **Print Image** off the menu bar to print the images to the select printer.

9.4 Printing Images in a Layout/Group/Series

The imaging application gives users the ability to print an entire layout or to select specific images in the layout for printing.

9.4.1 Printing an Entire Layout

9.4.1.1 View an existing patient's images and then double-click on the desired layout thumbnail to view the entire layout in full view.

9.4.1.2 Select **Print > Print Layout/Progression** off the menu bar.

9.4.1.3 The Wizard advances to the print utility.

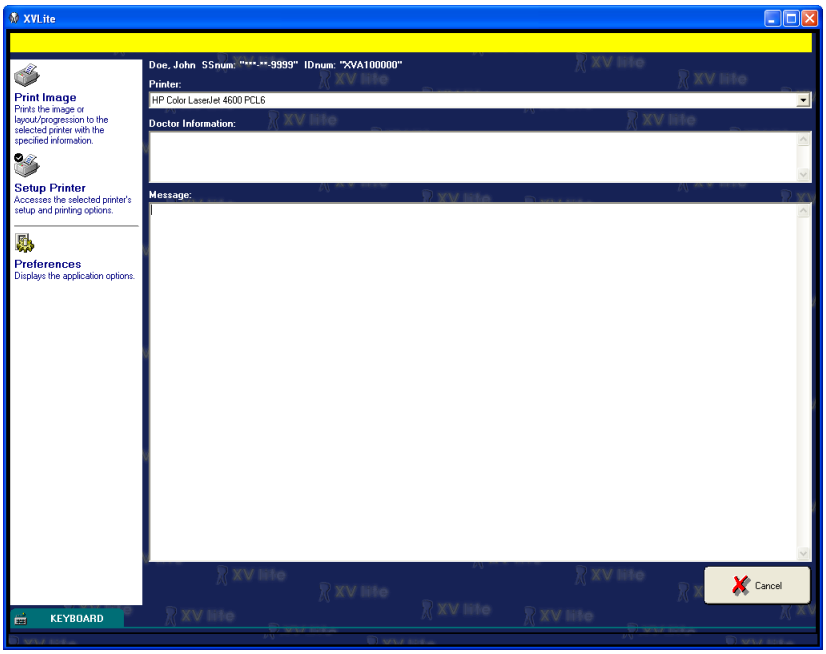

- Select the desired printer off the 'Printer' drop-down list.
- Complete the 'Doctor's Information' text box, if desired, that should be printed with the image.
- Complete the 'Message' text, if desired.

9.4.1.4 Select **Print Image** off the menu bar to print the layout to the select printer.

9.4.2 Printing One or More Images from a Layout

9.4.2.1 View an existing patient's images and then double-click on the desired layout thumbnail to view the entire layout in full view.

9.4.2.2 Select **Print > Print Layout/Progression** off the menu bar.

9.4.2.3 The Wizard advances to the layout print utility.

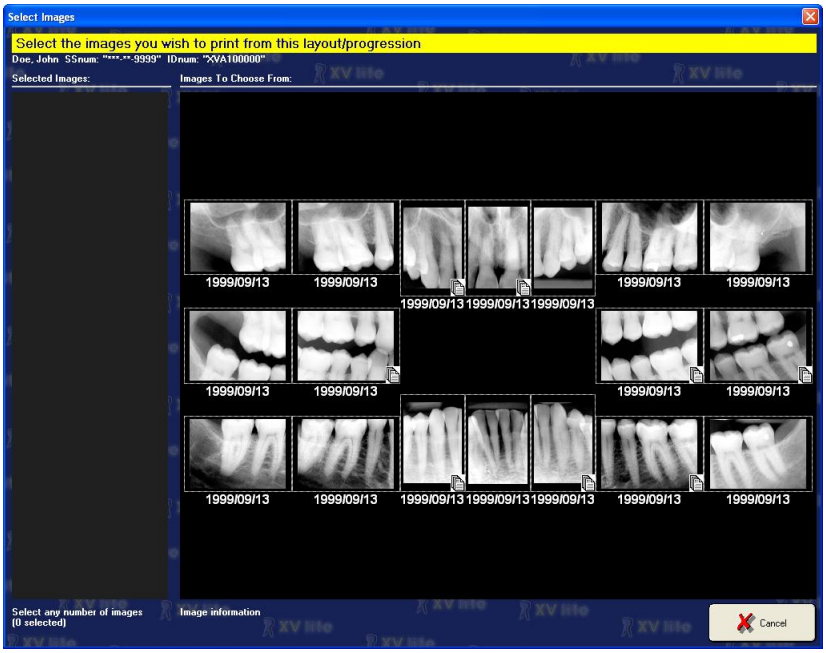

- The 'Images To Chose From' section on the right displays the current images in the patient's record. Click on each desired image to add to the print job.
- Each image that is added to the print job will display in the 'Selected Images' section on the left. If the wrong image is selected, click on it once to remove it.
- When ready to proceed with the print job, click on **OK**.

9.4.2.4 The Wizard advances to the multiple image print utility.

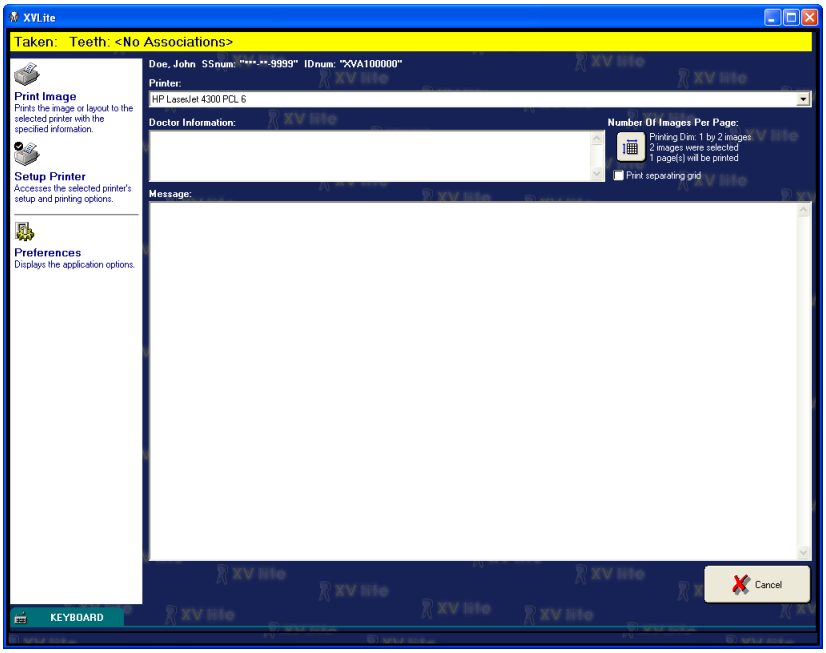

- Select the desired printer off the 'Printer' drop-down list.
- Complete the 'Doctor's Information' text box, if desired, that should be printed with the image.
- To the right, the 'Number of Images Per Page' section indicates the way the images will be printed on a grid and the total number of pages.

- Click on the button to reconfigure the layout of the print job. Use the mouse to select the desired number of columns and rows for the image grid.

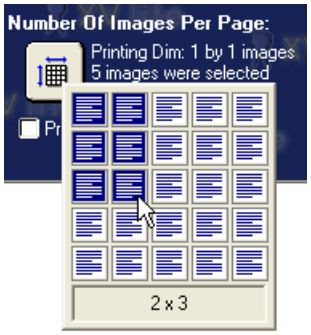

- Complete the 'Message' text, if desired.

9.4.2.5 Select **Print Image** off the menu bar to print the images to the select printer.

9.5 Document Templates

9.5.1 Overview

The imaging application provides a library of document templates (e.g. referral letters, treatment plans, clinical reports, image cards, etc.) that a user can select to automatically spawn a document in Microsoft® Word. Each template is embedded with codes that

insert an open patient's image(s) and select patient information (Name, ID number, SS Number, etc.) into a new document.

Macros must be enabled in Microsoft® Word in order to allow the execution of the Visual Basic codes embedded within the document templates. Apteryx, Inc. recommends setting the macro security level to Medium. The medium security setting permits a user to allow or disallow macros when working with documents. Refer to Microsoft's help documentation for further instructions.

9.5.2 Spawning Single Image Document Templates

9.5.2.1 View an existing patient's images; double-click on the desired image to view it in full view; and then select **Advanced Options** > **Document Templates** on the menu bar.

9.5.2.2 The first time the Document Template feature is utilized, the user is presented with the 'Document Template Options' dialog box to configure document handling settings. Refer to Appendix C: Configuring Document Handling Options for detailed instructions.

9.5.2.3 The 'Spawn Document' dialog box displays. Select the desired single-image document template to generate and click OK.

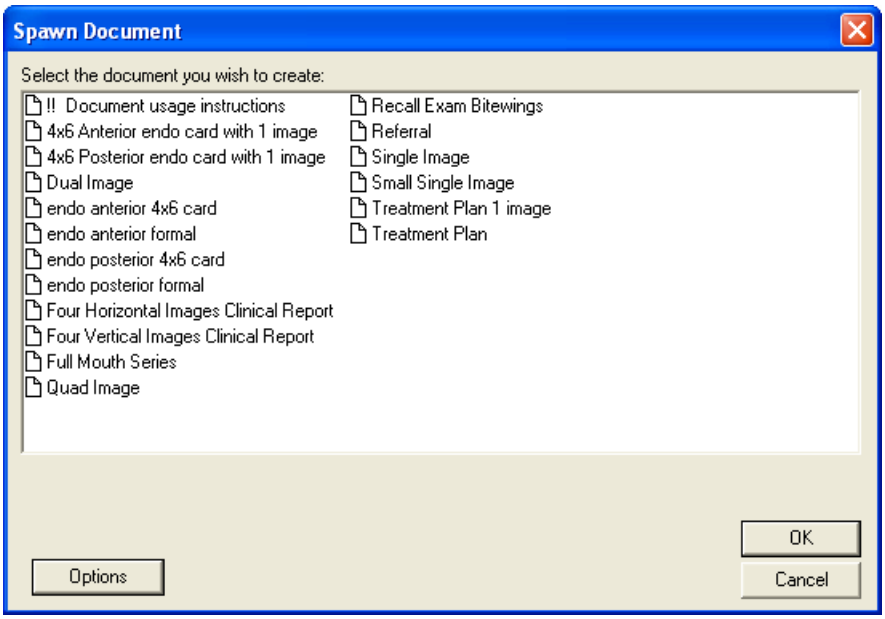

The naming convention of Apteryx-provided document templates typically indicates the document-type (i.e. Referral letter, treatment plan, etc.) and number of images the template can handle.

9.5.2.4 The imaging application will then proceed to launch Microsoft Word, embedding the image and patient information (outlined in green in the sample shown below) into a new word document.

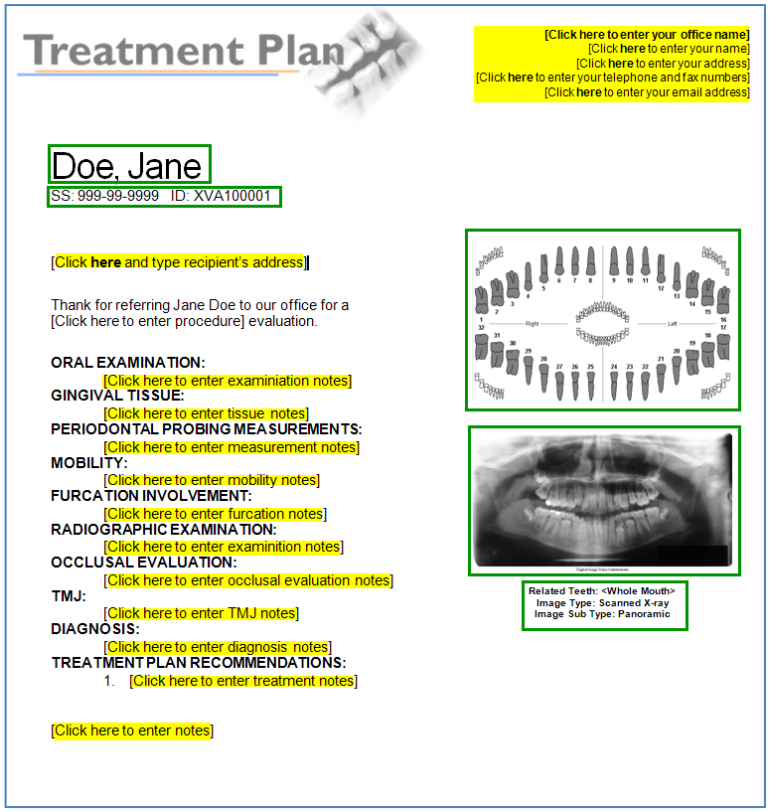
Treatment Plan
[Click here to enter your office name]
[Click here to enter your name]
[Click here to enter your address]
[Click here to enter your telephone and fax numbers]
[Click here to enter your email address]
Doe, Jane
SS: 999-99-9999 ID: XVA100001
[Click here and type recipient's address]
Thank for referring Jane Doe to our office for a [Click here to enter procedure] evaluation.
ORAL EXAMINATION:
[Click here to enter examiniation notes]
GINGIVAL TISSUE:
[Click here to enter tissue notes]
PERIODONTAL PROBING MEASUREMENTS:
[Click here to enter measurement notes]
MOBILITY:
[Click here to enter mobility notes]
FURCATION INVOLVEMENT:
[Click here to enter furcation notes]
RADIOGRAPHIC EXAMINATION:
[Click here to enter examinition notes]
OCCLUSAL EVALUATION:
[Click here to enter occlusal evaluation notes]
TMJ:
[Click here to enter TMJ notes]
DIAGNOSIS:
[Click here to enter diagnosis notes]
TREATMENT PLAN RECOMMENDATIONS:
1. [Click here to enter treatment notes]
[Click here to enter notes]
Related Teeth: <Whole Mouth>
Image Type: Scanned X-ray
Image Sub Type: Panoramic

9.5.2.5 Additional fields (highlighted in yellow in the sample above) can be manually typed in by the user to complete the document. Click on each field to enter the required information.

9.5.3 Spawning Multiple Image Document Templates

9.5.3.1 View an existing patient's images and then select **Spawn Multiple Image Document** off the menu bar.

9.5.3.2 The first time the Document Template feature is utilized, the user is presented with the 'Document Template Options' dialog box to configure document handling settings. Refer to Appendix C: Configuring Document Handling Options for detailed instructions.

9.5.3.3 The Wizard will advance to an image selection screen.

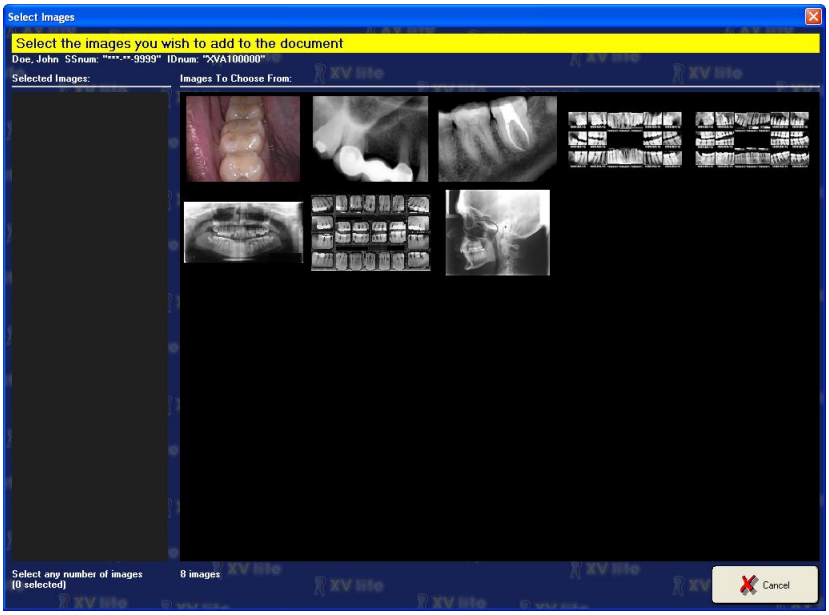
Select Images
Select the images you wish to add to the document
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Selected Images:
Images To Choose From:
Select any number of images (0 selected)
8 images
Cancel

- The 'Images To Chose From' section on the right displays the current images in the patient's record. Click on each desired image to add to the print job.
- Each image that is added to the print job will display in the 'Selected Images' section on the left. If the wrong image is selected, click on it once to remove it.
- When ready to proceed, click on **OK**.

9.5.3.4 The 'Spawn Document' dialog box displays. Select the desired single-image document template to generate and click **OK**.

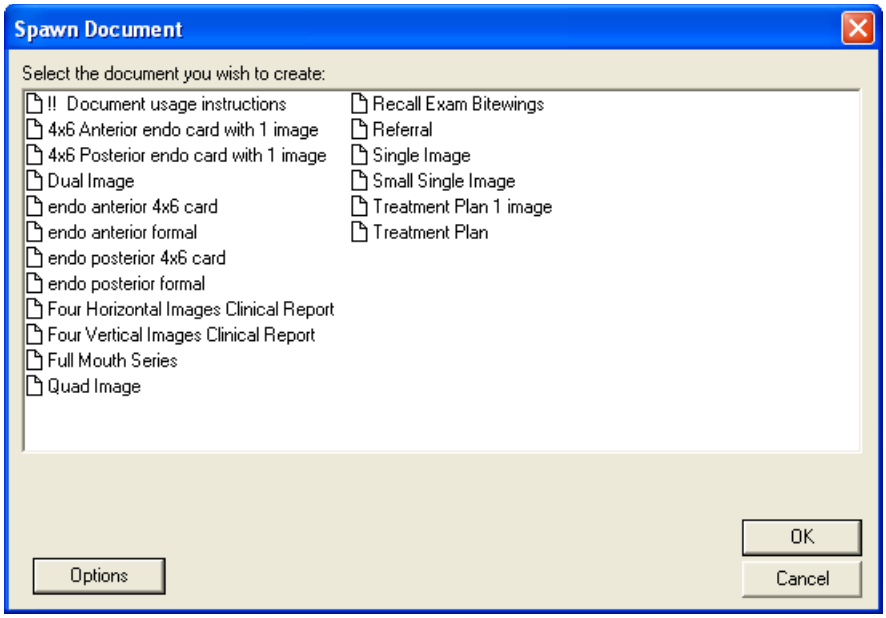

The listed document templates are not necessarily multiple-image templates. The naming convention of Apteryx-provided document templates typically indicates the document-type (i.e. Referral letter, treatment plan, etc.) and number of images the template can handle.

9.5.3.5 The imaging application will then proceed to launch Microsoft Word, embedding the images and patient information (outlined in green in the sample shown below) into a new word document.

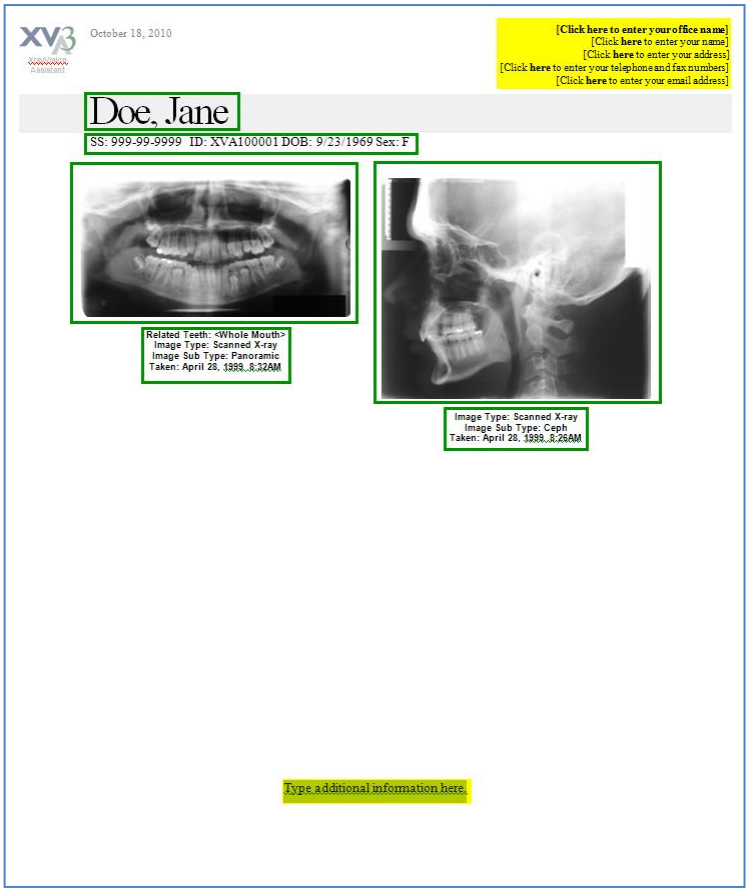
October 18, 2010
[Click here to enter your office name]
[Click here to enter your name]
[Click here to enter your address]
[Click here to enter your telephone and fax numbers]
[Click here to enter your email address]
Doe, Jane
SS: 999-99-9999 ID: XVA100001 DOB: 9/23/1969 Sex: F
Related Teeth: <Whole Mouth>
Image Type: Scanned X-ray
Image Sub Type: Panoramic
Taken: April 28, 1998, 8:32AM
Image Type: Scanned X-ray
Image Sub Type: Ceph
Taken: April 28, 1998, 8:26AM
Type additional information here.

9.5.3.6 Additional fields (highlighted in yellow in the sample above) can be manually typed in by the user to complete the document. Click on each field to enter the required information.

10 APPENDIX A: COMMON FUNCTIONS AND UTILITIES

10.1 Importing Images from an External Source

Digital images captured from digital cameras or other external sources are normally stored by the user in a known location on the local hard drive. The imaging application provides standard functionality that allows users to import and associate external files to a patient record:

This feature can be used to manually import one or more images (JPEGs, GIFs, TIFFs, etc.) into a patient record as single images or into a layout/group.

To import images:

10.1.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

10.1.2 Select the patient record and click on the **View Images** button on the menu bar.

10.1.3 The 'View Images for which teeth?' displays. Select **View Images For All Teeth**.

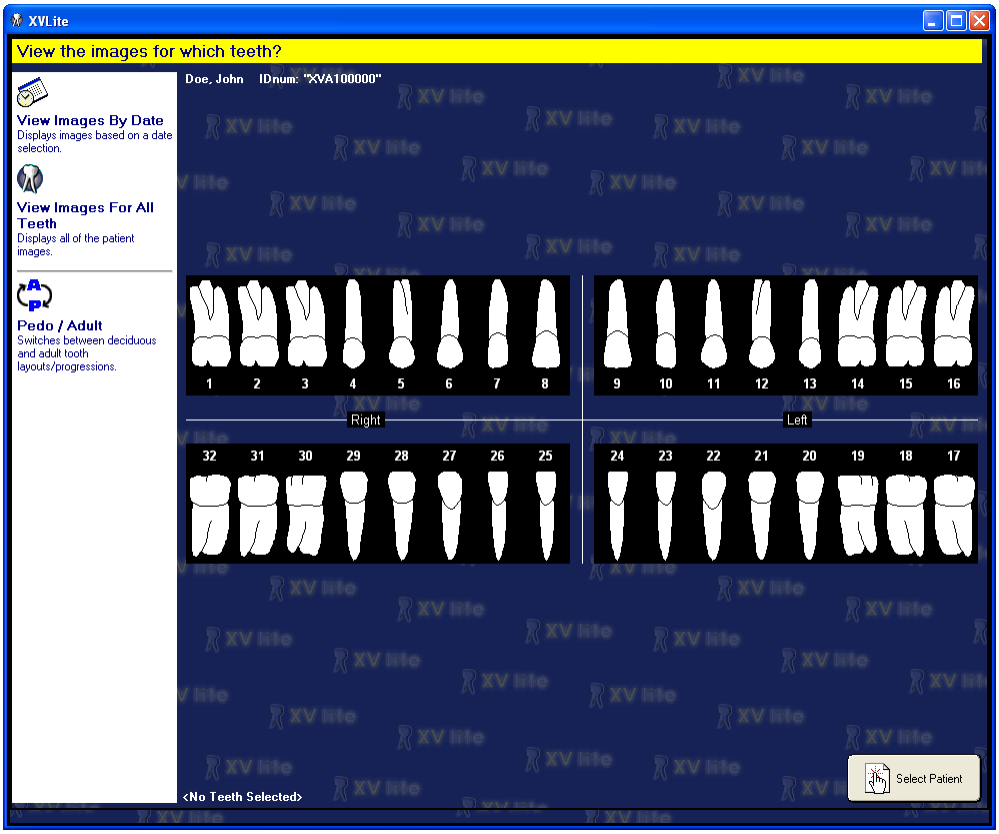
XVLite
View the images for which teeth?
Doe, John IDnum: "XVA100000"
View Images By Date
Displays images based on a date selection.
View Images For All Teeth
Displays all of the patient images.
Pedo / Adult
Switches between deciduous and adult tooth layouts/progressions.
1 2 3 4 5 6 7 8
9 10 11 12 13 14 15 16
Right
Left
32 31 30 29 28 27 26 25
24 23 22 21 20 19 18 17
Select Patient
<No Teeth Selected>

10.1.4 A screen displaying thumbnails of the patient's images displays. Select **Import Images**.

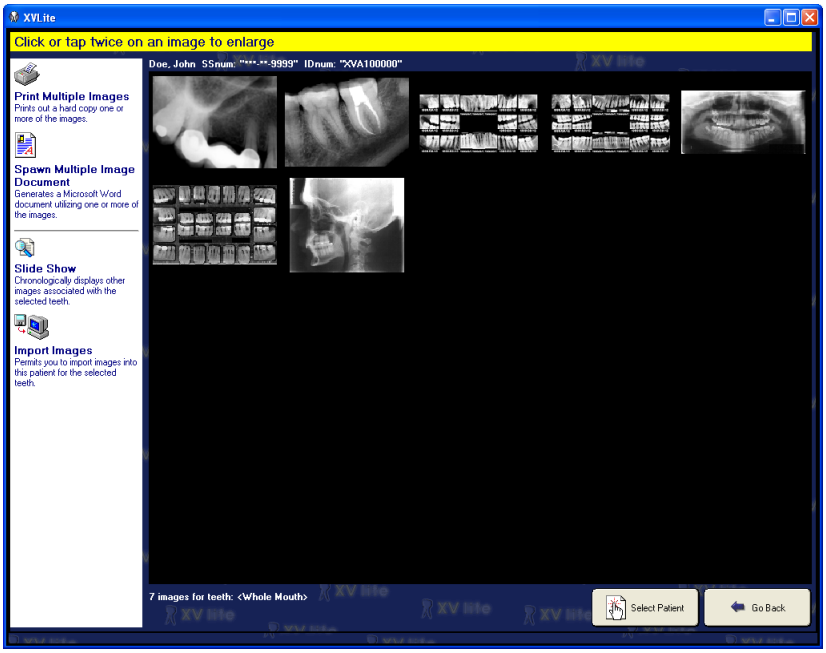
XVLite
Click or tap twice on an image to enlarge
Doe, John SSnum: "***-**-9999" IDnum: "XVA100000"
Print Multiple Images
Prints out a hard copy one or more of the images.
Spawn Multiple Image Document
Generates a Microsoft Word document utilizing one or more of the images.
Slide Show
Chronologically displays other images associated with the selected teeth.
Import Images
Permits you to import images into this patient for the selected teeth.
7 images for teeth: <Whole Mouth>
Select Patient
Go Back

10.1.5 The 'Open' dialog box will display. Browse to the known location/directory where the image(s) is stored and click on it once. To select more than one, hold down the control button and select each additional image. Click on **Open** when done.

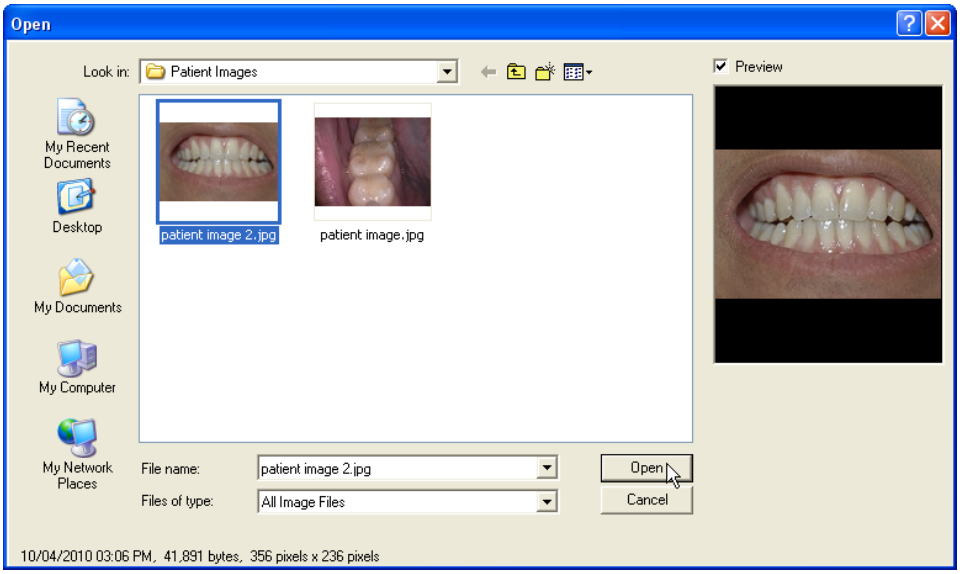

10.1.6 The 'Move files to patient' dialog box displays. Enable the option to delete the original file after the move, if desired. Click the **Yes …** button to proceed with the move.

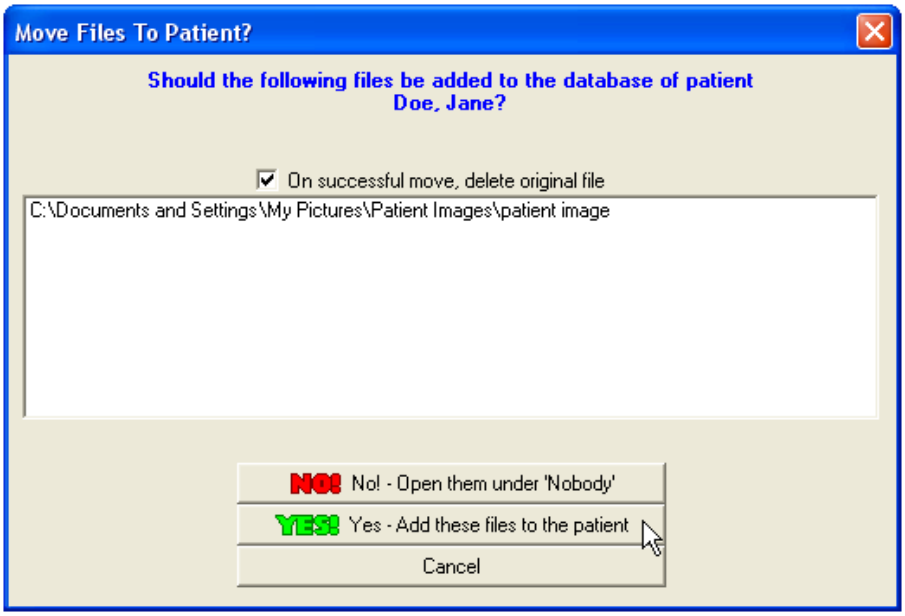
Move Files To Patient?
Should the following files be added to the database of patient
Doe, Jane?
On successful move, delete original file
C:\Documents and Settings\My Pictures\Patient Images\patient image
NO! No! - Open them under 'Nobody'
YES! Yes - Add these files to the patient
Cancel

10.1.7 If the option to delete the original file after the move has been selected, the 'Delete Original Files' dialog box displays. Click **Yes** to delete the image(s) if desired.

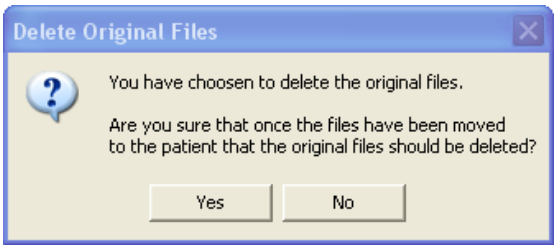
Delete Original Files
You have choosen to delete the original files.
Are you sure that once the files have been moved
to the patient that the original files should be deleted?
Yes
No

10.1.8 The imported image(s) will display in the imaging application complete and will be automatically stored to the patient's file.

10.2 Deleting a Patient's Images

Follow the steps below to remove one or more images from a patient's file:

10.2.1 Enter the patient's information in one or more fields of the search utility or scroll down to find the desired patient record.

10.2.2 Select the patient's record and then select **Advanced Patient Options > Delete Patient Images** on the menu bar.

10.2.3 The 'Delete Patient Image Files' dialog box opens, displaying thumbnails of all the patient's images. Select one or more of the desired images and click on the **Delete** button.

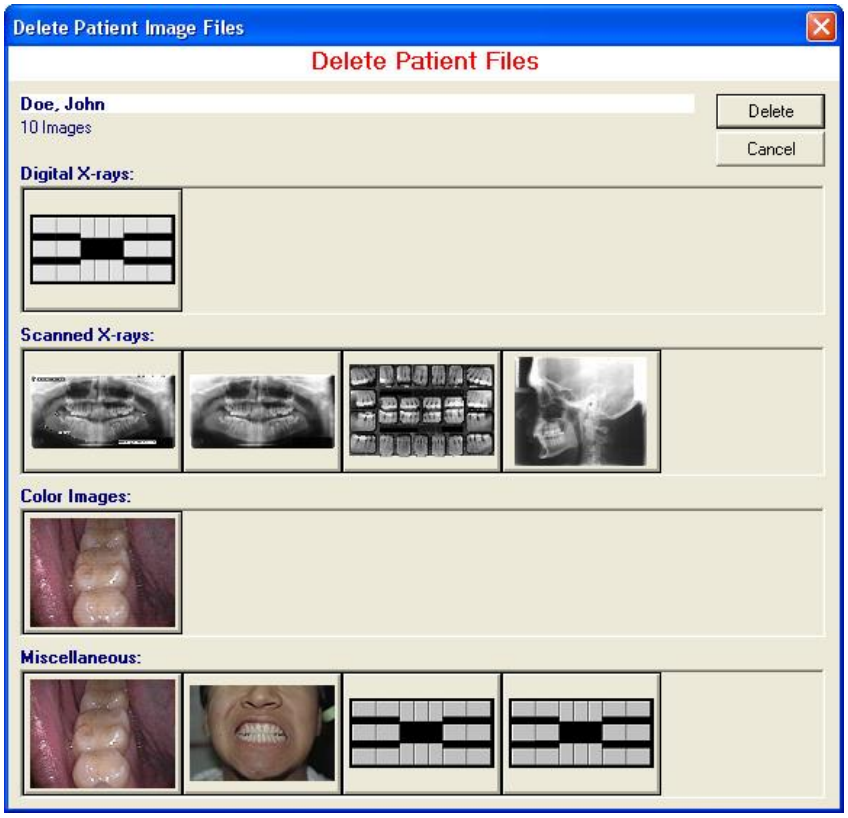

10.2.4 The following warning messages display. If sure, select **Yes** on each to continue with the deletion.

10.2.4.1

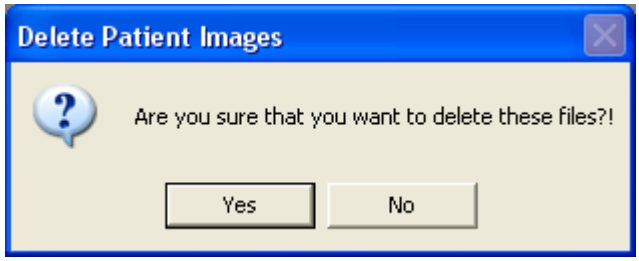

10.2.4.2

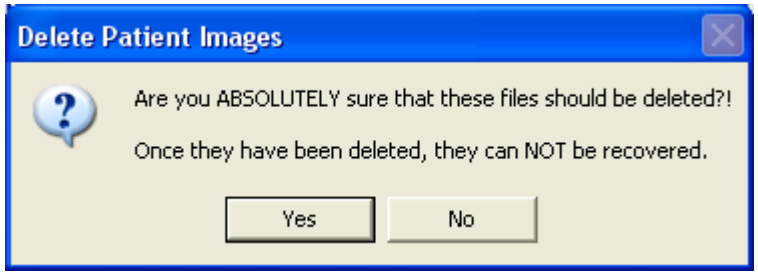
Delete Patient Images
Are you ABSOLUTELY sure that these files should be deleted?!
Once they have been deleted, they can NOT be recovered.
Yes
No

10.3 Finding Images by Date

10.3.1 Overview

Occasionally, users may need to perform a search for an image that was inadvertently captured under the wrong patient. The 'Find Images by Date' utility gives users the ability

to search the entire patient database for all images captured within a specified date range.

10.3.2 Performing a Search

10.3.2.1 Select **Preferences** off the main menu bar. After the wizard advances, select **Database** and then click **Find Images By Date**.

10.3.2.2 The 'Find Images by Date' dialog box displays.

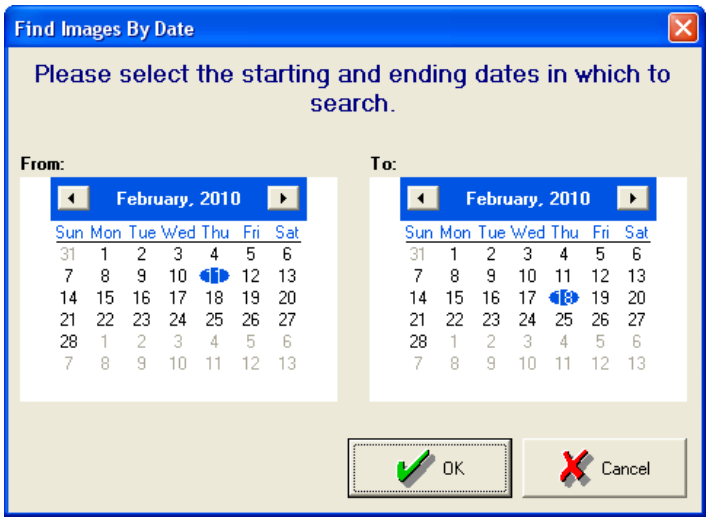

- Use the 'From' and 'To' calendars to specify an application date range to perform a search.
- Click on the **OK** button to proceed with the search.

10.3.2.3 The 'Found Images' dialog box displays if there are images in the patient database that match the search criteria.

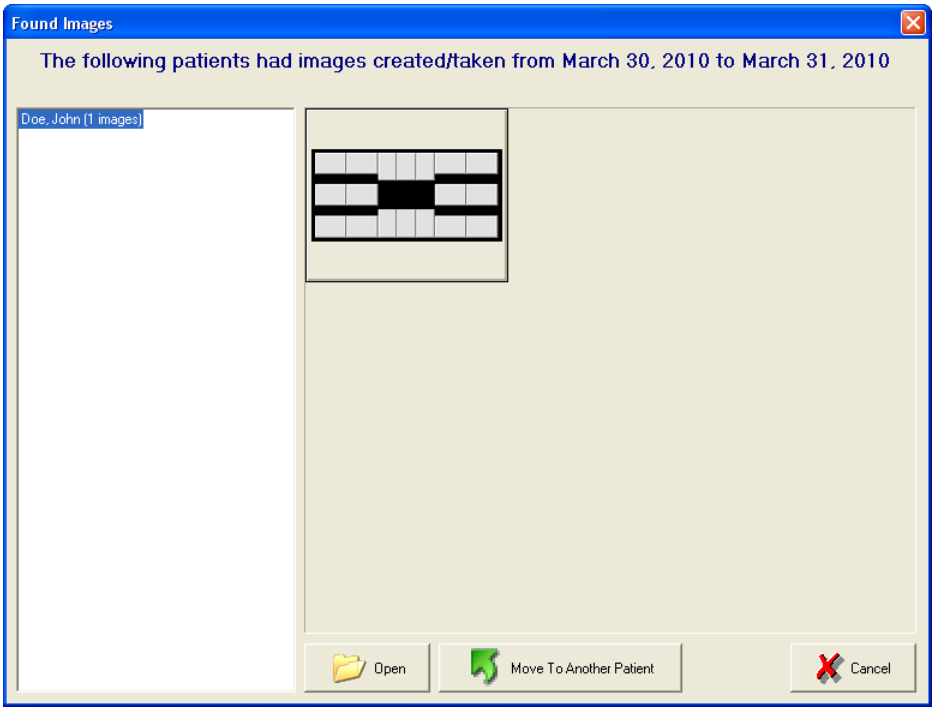
Found Images
The following patients had images created/taken from March 30, 2010 to March 31, 2010
Doe, John (1 images)
Open
Move To Another Patient
Cancel

- Select a patient on the left column to preview their related images.
- If the desired image is found, click **Open** to view it … OR … click on **Move to Another Patient** to transfer the image to the correct patient.

10.3.2.4 If **Move to Another Patient** was selected in the previous step, The 'Move Layout to Patient' utility displays. Select the patient from the list to which the layout is to be moved and click on the **OK** button.

11 APPENDIX B: CUSTOMIZING LAYOUT DEFINITIONS

11.1 General Information

A layout is a patented method of displaying a series of images in a single workspace. The imaging application comes equipped with pre-defined layouts that a dental practice can use to capture patient images for bitewings (2 and 4 BWXs), full mouth series (18 and 22 FMXs), anteriors (upper and lower), etc.

Each layout has a series of free-floating tiles that are arranged to be a representation of the anatomical location of groups of teeth in a mouth. Each tile in a layout identifies the source of the image (sensor, scanner, video, etc.), its orientation, related tooth associations, and its order in the capture series.

11.2 Overview of the 'Layout Definition' Dialog Box

The 'Layout Definition' dialog box is where users can customize their own layouts by creating new or modifying the definitions in an existing layout to meet their needs.

11.2.1 Accessing Layout Definitions

11.2.1.1 Select any patient record and click on the **Take X-ray** button on the menu bar. The wizard advances to the 'Take X-rays for which teeth? …' screen. Select **Take an Automated X-ray Series**.

11.2.1.2 The wizard will advance to a layout selection screen. Click on the **Customize Layouts** button. The 'Layout Definitions' dialog box will display.

11.2.2 The 'Layout Definitions' Interface

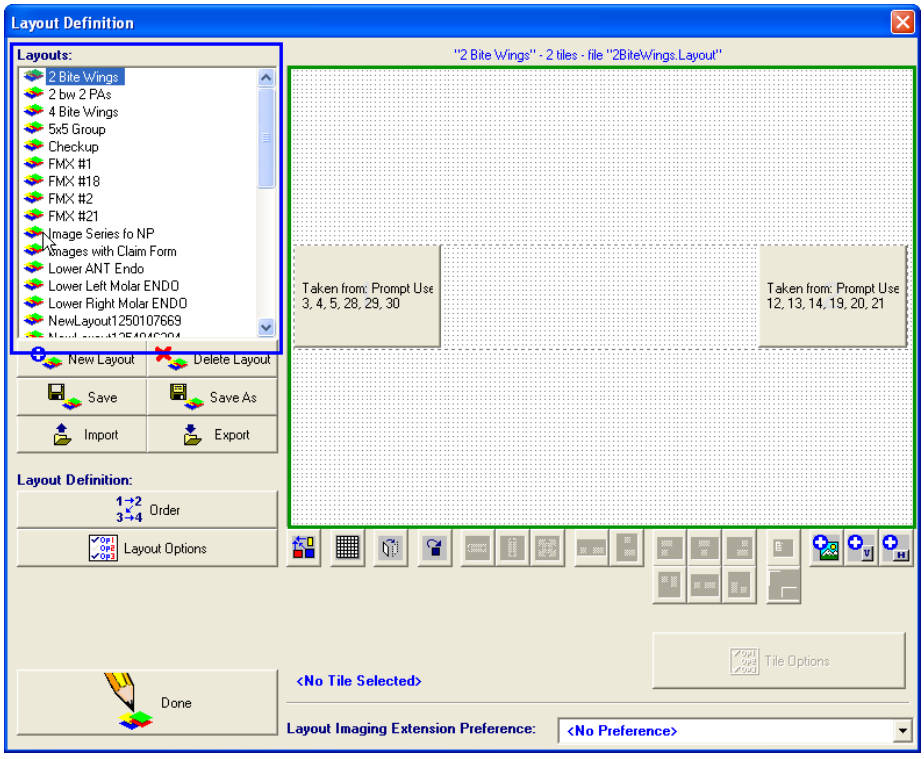

11.2.2.1 All existing layouts are listed in the 'Layouts' section (outlined in blue above).

11.2.2.2 If a layout is selected, it will display in edit mode in the large preview window (outlined in green above).

11.2.3 Layout Options

Users can configure general layout options when creating a new layout or editing an existing layout (selecting the Layout Options button). The layout options dialog box is displayed in 'Edit Layout' mode below.

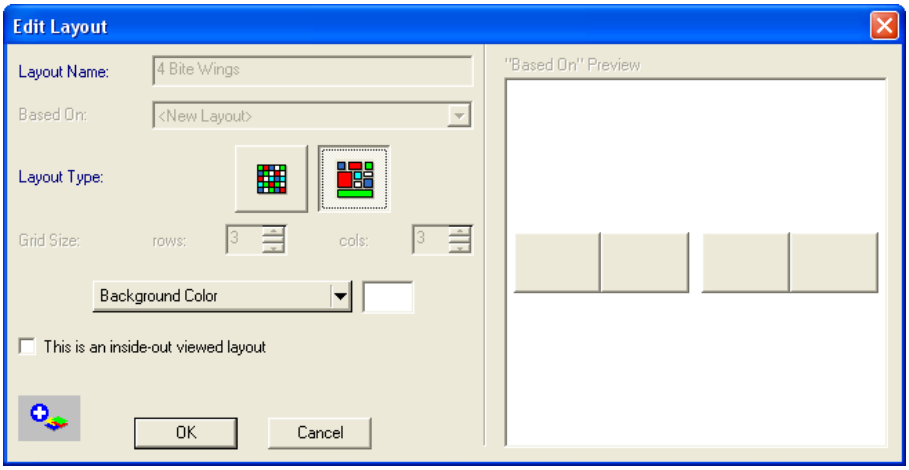

Users can define/redefine the follow general layout options:

- 'Layout Type' – Users can select between a grid-type with static tiles ( ) … OR … a layout with free-floating tiles ( ).
- 'Grid-Size' – If the grid is selected as 'layout type', the user can specify the amount of rows and columns in the grid.
- Background Color – Users can select the drop-down to specify a different color for the layout background.
- 'This is an inside-out viewed layout' – This option can be enabled to define the layout as being viewed from inside out. Images acquired will be automatically flipped inside-out in this mode.

11.2.4 The 'Layout Definitions' Toolbar

There is a collection of buttons below the preview window that can be used to configure the layout/tiles of a selected layout as desired. Some buttons will remain grayed out until a tile or tiles are selected. Refer to the table below for a quick description of each.

	Recovers "lost" tiles (caused by modifications that cause tiles to disappear from preview).		Adjusts height of selected tiles to equal length.		Aligns the center of selected tiles.		Generates a duplicate of the selected tile.
	Forces tiles to snap to a defined grid		Adjusts height & width of selected tiles to equal length.		Aligns the right-hand edge of selected tiles.		Rotates the selected tile.
	Flips entire layout horizontally (inside-out view)		Evenly spaces selected tiles horizontally.		Aligns the top edge of selected tiles.		Adds a new tile to the layout.

	Sets layout tile source (video, sensor, etc.)		Evenly spaces selected tiles vertically.		Aligns the middle of selected tiles.		Adds a vertical tile to the layout.
	Adjusts width of selected tiles to equal length.		Aligns the left-hand edge of selected tiles.		Aligns the bottom edge of selected tiles.		Adds a horizontal tile to the layout.

11.3 Common Layout Tasks: Changing the Capture Order

Each tile in a layout identifies the source of the image (sensor, scanner, video, etc.), its orientation, related tooth associations, and its order in the capture series. To change the capture order:

11.3.1 Select the desired layout to edit. The layout/tiles display in the preview window.

11.3.2 Select the Order button to enable the tile ordering function.

11.3.3 Note that the current capture order of each tile displays in the top-left corner of each tile.

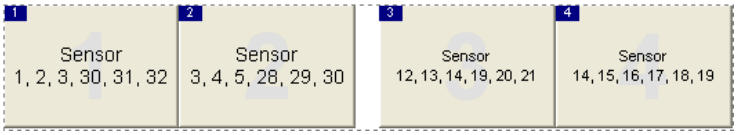

11.3.4 With the ordering function now enabled, click on each tile in the order desired for capturing. The tile numbers will be reordered as the user selects each tile in the series.

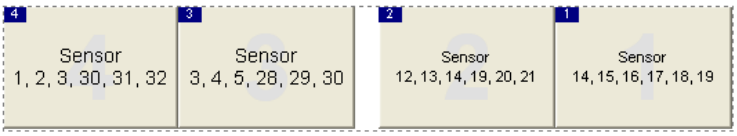

11.3.5 Select the **Save** button to store the changes.

11.4 Common Layout Tasks: Changing the Capture Source

Each tile in a layout identifies the source of the image (sensor, scanner, video, etc.), its orientation, related tooth associations, and its order in the capture series. To modify the capture source of a layout:

11.4.1 Select the desired layout to edit. The layout/tiles display in the preview window.

11.4.2 Select the source button ( ) from the toolbar below the preview window.

11.4.3 The 'Take From' dialog box displays.

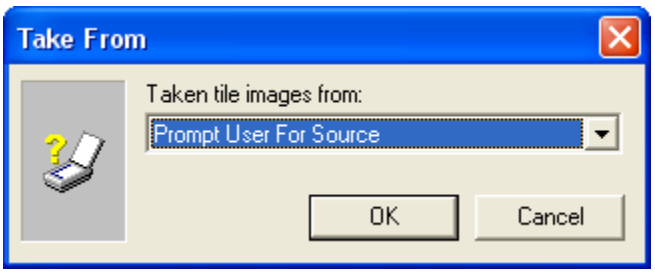

11.4.4 Select the desired source from the provided drop-down list:

- **Prompt User For Source** – If selected the user will be prompted to select a source during the layout capture process.
- **Nowhere** – If selected, the user will not be prompted for any source.
- **Scanner** – If selected, the layout will be setup to acquire phosphor plates scanners, etc.
- **Sensor**– If selected, the layout will be ready to acquire from x-ray sensors.
- **File** – If selected, the layout will be setup to acquire images from the local hard drive, network, or media device attached to the computer.
- **Clipboard**– If selected, the layout will be setup to acquire an image stored in the computer's memory via the <copy> function.
- **TWAIN Device** - If selected, the layout will be setup to acquire from devices, such as document scanners, that have the manufacturer's TWAIN drivers installed on the computer.
- **Video Source** - If selected, the layout will be setup to acquire from a video source, such as an intra-oral or extra-oral camera, using the DirectVideo or Real-Time Video extension.
- **Auto-Import** - If selected, the layout will be setup to acquire using the Auto-Import utility.

11.4.5 Click **OK** when done.

Select the **Save** button on the 'Layout Definitions' dialog box to store the changes.

11.5 Common Layout Tasks: Adding Tiles

Each tile in a layout identifies the source of the image (sensor, scanner, video, etc.), its orientation, related tooth associations, and its order in the capture series. To add an additional tile to a layout:

11.5.1 Select the desired layout to edit. The layout/tiles display in the preview window.

11.5.2 From the toolbar below the preview window, select to add a horizontal tile … OR … to add a vertical tile to the layout.

11.5.3 Refer to The 'Layout Definitions' Toolbar section above for additional functions that can be performed to further configure the tile as needed.

11.6 Common Layout Tasks: Creating New Layouts Based on Existing Layouts

The imaging application gives users the ability to create a layout from scratch or to create a new layout based on an existing layout. Basing a new layout on an existing one is a useful if needing to create a duplicate layout for different hardware. For example, if a user has an existing 4 Bitewing Layout on the 'Layout Definition' screen that is set to capture from a sensor, a duplicate layout can be easily created and set to capture from their intra-oral camera, if needed.

To create a new layout based on an existing layout:

11.6.1 Select the **New Layout** button. The 'New Layout' dialog box displays.

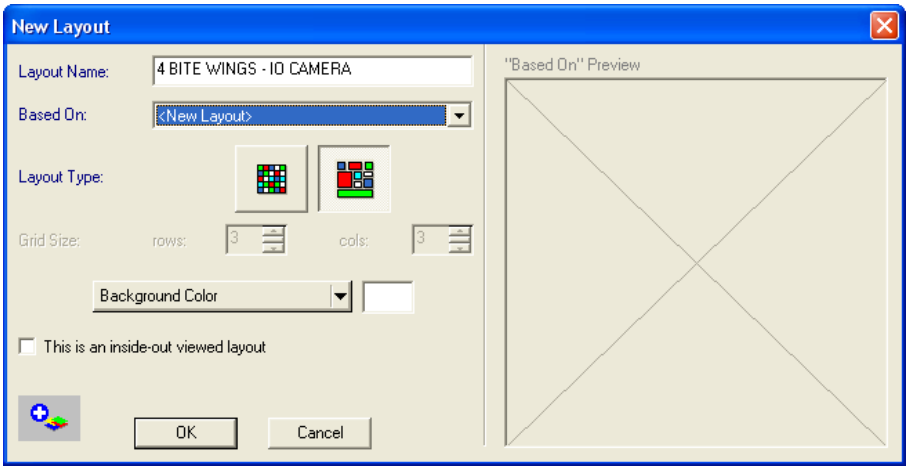

11.6.2 Enter a descriptive name for the new layout in the 'Layout Name' field.

11.6.3 Click on the 'Based On' drop-down list to select the desired layout the new one being created will be based on.

When creating a new custom layout from scratch, using the Layout Type of grid is limited compared to free-floating. Accordingly, free-floating is the preferred Layout Type for creating a custom layout.

12 APPENDIX C: CONFIGURING DOCUMENT HANDLING OPTIONS

12.1 Overview

The imaging application provides a library of document templates (e.g. referral letters, treatment plans, clinical reports, image cards, etc.) that a user can select to automatically spawn a document in Microsoft® Word. Each template is embedded with codes that insert an open patient's image(s) and select patient information (Name, ID number, SS Number, etc.) into a new document.

Macros must be enabled in Microsoft® Word in order to allow the execution of the Visual Basic codes embedded within the document templates. Apteryx, Inc. recommends setting the macro security level to Medium. The medium security setting permits a user to allow or disallow macros when working with documents. Refer to Microsoft's help documentation for further instructions.

12.2 Configuring Document Template Options

12.2.1 The first time the Document Template feature is utilized to spawn single image document templates or multiple image document templates in Microsoft® Word, the user is presented with the 'Document Template Options' dialog box to configure document handling settings.

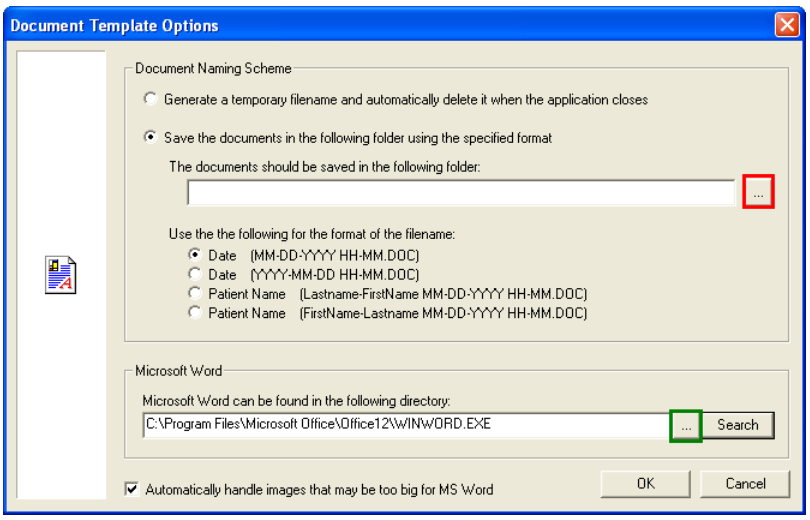
Document Template Options
Document Naming Scheme
Generate a temporary filename and automatically delete it when the application closes
Save the documents in the following folder using the specified format
The documents should be saved in the following folder:
...
Use the the following for the format of the filename:
Date (MM-DD-YYYY HH-MM.DOC)
Date (YYYY-MM-DD HH-MM.DOC)
Patient Name (Lastname-FirstName MM-DD-YYYY HH-MM.DOC)
Patient Name (FirstName-Lastname MM-DD-YYYY HH-MM.DOC)
Microsoft Word
Microsoft Word can be found in the following directory:
C:\Program Files\Microsoft Office\Office12\WINWORD.EXE
...
Search
Automatically handle images that may be too big for MS Word
OK
Cancel

12.2.2 By default, documents are created as temporary documents that will be deleted once Microsoft® Word is closed. Select **Save the documents in the document in following folder …** to specify a specific location on the computer to store spawned documents.

12.2.3 Click on the browse button (outlined in red above). The Select Path' dialog box displays.

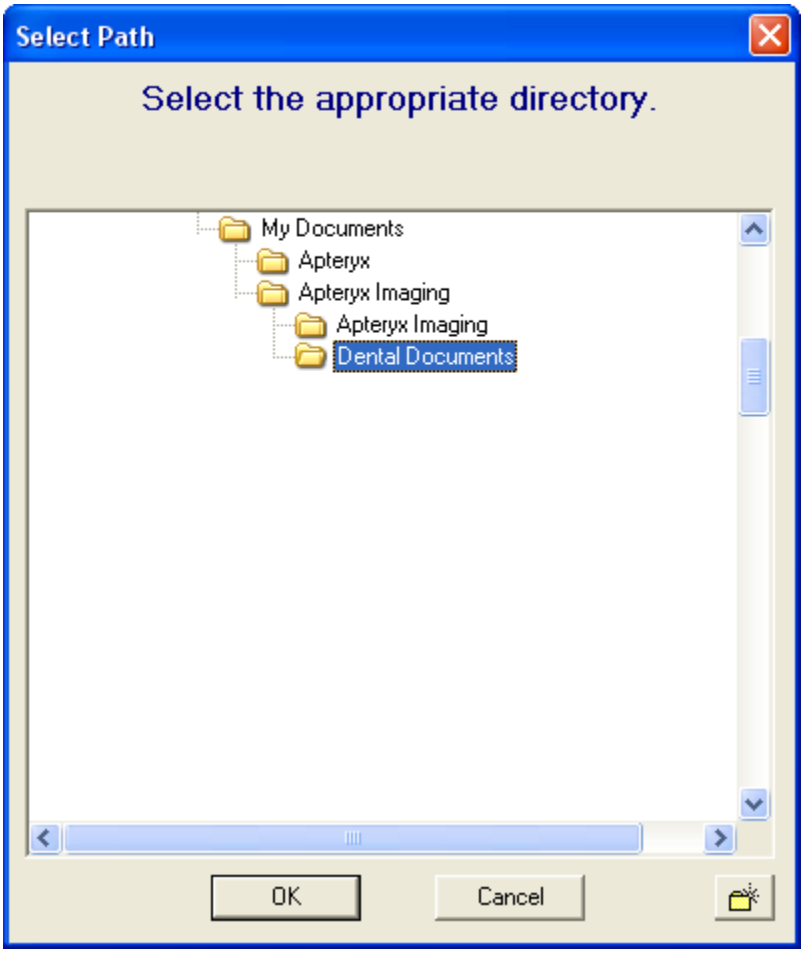

12.2.3.1 Use the directory tree to find and select the appropriate folder.

12.2.3.2 Click **OK** to return to the 'Document Options' dialog box.

12.2.4 Select the desired naming scheme to use for any Word document spawned from the imaging application.

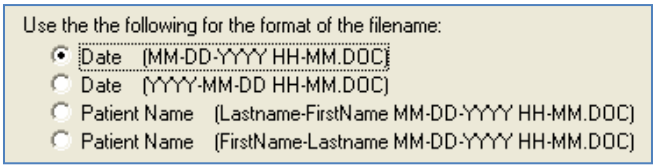
Use the the following for the format of the filename:
Date (MM-DD-YYYY HH-MM.DOC)
Date (YYYY-MM-DD HH-MM.DOC)
Patient Name (Lastname-FirstName MM-DD-YYYY HH-MM.DOC)
Patient Name (FirstName-Lastname MM-DD-YYYY HH-MM.DOC)

12.2.5 Select the option to 'Automatically handle images that may be too big for MS Word'. If enabled, large images will be automatically resized to fit within the document's designated area for embedded images.

12.2.6 Before Microsoft® Word can be used to create documents; the location of the application must be configured. To specify the location of Microsoft Word on the computer, click the browse button (outlined in green above) to manually search for the Microsoft Word executable (typically called WINWORD.EXE) … OR … click the **Search** button to have the software find the executable.

12.2.7 Click **OK** to save the changes and continue with the process.

13 APPENDIX D: CONFIGURING PREFERENCES

13.1 General Information

The imaging application is a customizable application that can be fined tuned to suit a user's needs. These options can be accessed by clicking on Preferences on the main menu bar. The following section describes the available options on the 'Preferences' screen.

13.2 General Preferences

Select General off the menu bar to display options related to the general functionality or operability of the imaging application.

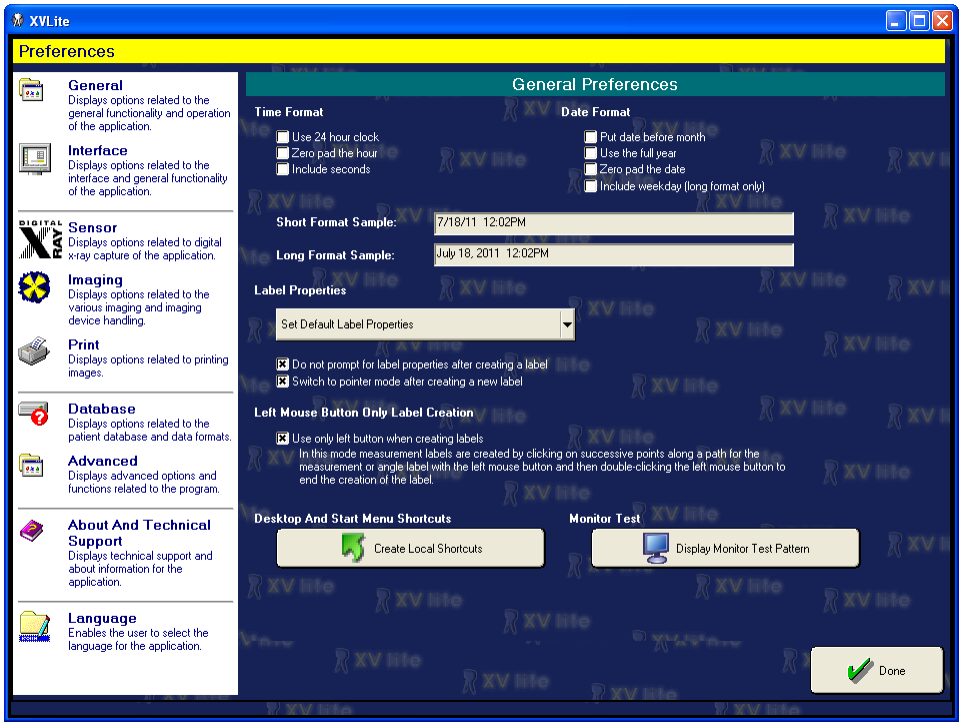
XVLite
Preferences
General
Displays options related to the general functionality and operation of the application.
Interface
Displays options related to the interface and general functionality of the application.
Sensor
Displays options related to digital x-ray capture of the application.
Imaging
Displays options related to the various imaging and imaging device handling.
Print
Displays options related to printing images.
Database
Displays options related to the patient database and data formats.
Advanced
Displays advanced options and functions related to the program.
About And Technical Support
Displays technical support and about information for the application.
Language
Enables the user to select the language for the application.
General Preferences
Time Format
Use 24 hour clock
Zero pad the hour
Include seconds
Date Format
Put date before month
Use the full year
Zero pad the date
Include weekday (long format only)
Short Format Sample:
7/18/11 12:02PM
Long Format Sample:
July 18, 2011 12:02PM
Label Properties
Set Default Label Properties
Do not prompt for label properties after creating a label
Switch to pointer mode after creating a new label
Left Mouse Button Only Label Creation
Use only left button when creating labels
In this mode measurement labels are created by clicking on successive points along a path for the measurement or angle label with the left mouse button and then double-clicking the left mouse button to end the creation of the label.
Desktop And Start Menu Shortcuts
Create Local Shortcuts
Monitor Test
Display Monitor Test Pattern
Done

- 'Time Format':
  - **Use 24 hour clock** - Time reads out in military time. 9:50 PM would be 21:50
  - **Zero pad the hour** - Places a "0" in front of the hour. So 9:50 PM would read 09:50 PM
  - **Include seconds** - Places seconds at the end of the time. 9:50 PM would read 9:50:45 PM
- 'Date Format':
  - **Put date before month** - Places the date before the month as they do in Europe. Instead of August 14th it would read 14th August
  - **Use the full year** - Instead of placing "00" it would read "2000"
  - Zero pad the date - Places a "0" in front of the date if it is less than 10
  - **Include weekday (long format only)** - Includes the day of the week (e.g. Monday, Tuesday, etc.) in long format.

- 'Label Properties':
  - Click the **Set Default Label Properties** to set the default formatting of common labels and markers such as Angles, Arrows, etc. A related properties dialog box will appear allowing users to configure pen size, pen color, fill color etc.
  - **Do not prompt for label properties after creating a label** – If selected, the label properties dialog box will be suppressed with adding labels, markers, or annotations. The defaults set here will always be applied.
  - **Switch to pointer mode after creating a new label** – If selected, the mouse will return to pointer mode rather than remaining in the mode of the selected label.

13.3 Interface Preferences

The 'Interface Preferences screen contains settings that control the appearance of the user interface and information displayed.

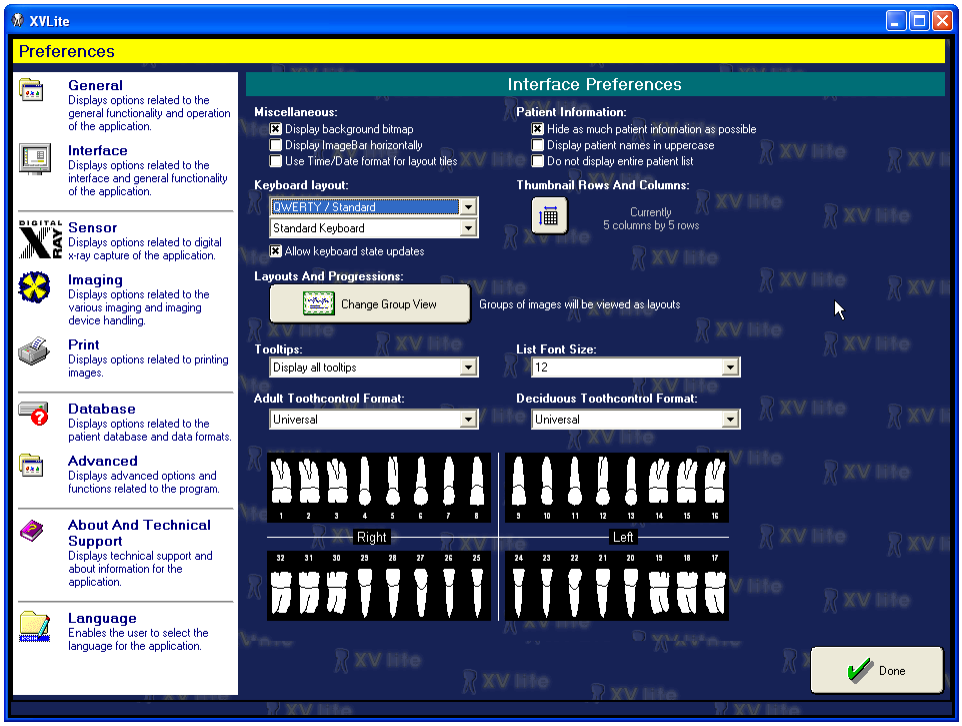

- 'Miscellaneous':
  - **Display background bitmap** – If disabled, the background image of the application will be removed.
  - **Display ImageBar horizontally** – Displays the Imagebar horizontally across the user interface.

    The ImageBar feature is typically enabled in NameGrabber, Apteryx's practice management bridging application, to display a patient's images in a floating bar. If utilizing a bridging mechanism built into a practice management application, the imagebar feature can be enabled within the imaging application by selecting any patient on the main interface and then clicking on Advanced Patient Options > Imagebar off the menu bar.
  - **Use time/date format for layout tile dates** – If disabled, the date displayed below layout tiles will appear in the *YYYY/MM/DD* format.

- 'Patient Information':
  - **Hide as much patient information as possible** - This option will hide SS numbers from the open patient index.
  - **Display patient names in uppercase** - Patient names are displayed in uppercase format when enabled.
  - **Do not display entire patient list** – If enabled the patient list on the main screen does not present an index of all patients. Only patients that match the search criteria as it is being entered will be displayed.
- 'Keyboard Layout':
  - Indicates what keyboard style and type are to be used for the on-screen keyboard that can be displayed on the various screens throughout the application. The default option, **QWERTY/Standard** is the standard U.S. setting. Select one of the various international keyboards supported by the application.
  - The Block and Standard settings indicate the key arrangement that is to be used when the keys are displayed. The Standard setting displays the keys in the standard keyboard configuration while the Block format rearranges the keys so that they may be easier to use in some wall mounted displays.
- 'Layouts And Progressions':
  - Select **Change Group View** to select a viewing preference (Layouts vs. Progressions) for image groups/series.
- 'Tooltips': Tooltips provide a description of the operation associated with a button that the cursor is hovering over. By default, the application is enabled to display all tooltips.
- 'List Font Size': Select an appropriate value off the drop list to increase the font size of the Patient List on the main screen.
- 'Adult Toothcontrol Format': allows users to set up the way the adult tooth control palettes are displayed. Options include:
  - **British**
  - **International** - 4 quadrants, 8 tooth forms (1-1, 1-2, 1-3, etc.)
  - **Universal** – Teeth numbers 1-32
- 'Deciduous Toothcontrol Format': allows users to set up the way the adult tooth control palettes are displayed. Options include:
  - **British**
  - **Palmer** - 4 quadrant, 5 tooth by letter (1-a, 1-b, 1-c)
  - **International** - 4 quadrants, 5 tooth by # (5-1, 5-2, 5-3)
  - **Universal** – Letters A-T

13.4 Sensor Preferences

Users can access the specific settings of installed sensor extensions, add new sensor definition or configuration files, and configure general sensor capture settings that apply to all sensors. Users can also configure audible indicators for sensor readiness and failure.

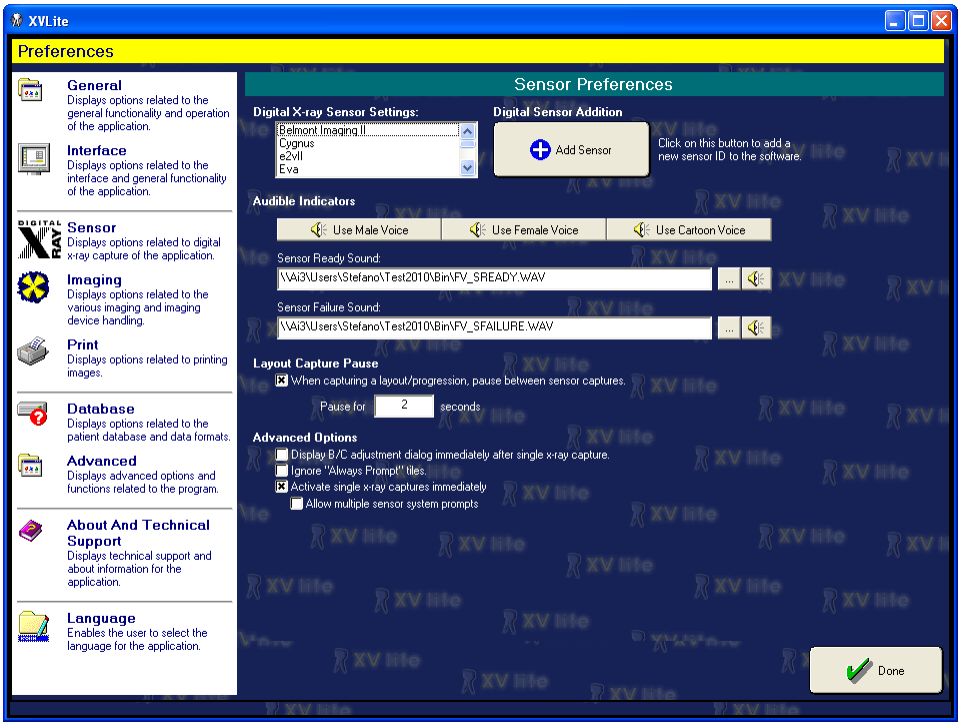
XVLite
Preferences
General
Displays options related to the general functionality and operation of the application.
Interface
Displays options related to the interface and general functionality of the application.
Sensor
Displays options related to digital x-ray capture of the application.
Imaging
Displays options related to the various imaging and imaging device handling.
Print
Displays options related to printing images.
Database
Displays options related to the patient database and data formats.
Advanced
Displays advanced options and functions related to the program.
About And Technical Support
Displays technical support and about information for the application.
Language
Enables the user to select the language for the application.
Sensor Preferences
Digital X-ray Sensor Settings:
Belmont Imaging II
Cygnus
e2vII
Eva
Digital Sensor Addition
Add Sensor
Click on this button to add a new sensor ID to the software.
Audible Indicators
Use Male Voice
Use Female Voice
Use Cartoon Voice
Sensor Ready Sound:
\\Ai3\Users\Stefano\Test2010\Bin\FV_SREADY.WAV
Sensor Failure Sound:
\\Ai3\Users\Stefano\Test2010\Bin\FV_SFAILURE.WAV
Layout Capture Pause
When capturing a layout/progression, pause between sensor captures.
Pause for 2 seconds
Advanced Options
Display B/C adjustment dialog immediately after single x-ray capture.
Ignore "Always Prompt" tiles.
Activate single x-ray captures immediately
Allow multiple sensor system prompts
Done

- 'Digital X-ray Sensor Settings': Lists the currently installed sensor extensions. Double-click an entry to access the sensor extension settings for post-capture filtration and other sensor-specific settings.
- 'Digital Sensor Addition' – Depending on the manufacturer's specifications, a sensor definition or configuration file (calibration, correction, or Gain file) may need to be added for the digital x-ray system. Select **Add Sensor** to add new sensor definitions to the software.

  Not all digital x-ray systems require the addition of sensor files for their digital sensors. Please consult the documentation that came with the system to see if the system requires sensor definition files to be loaded into the software.

- 'Audible Indicators' – The available options enable an audible voice that will say "Sensor Ready" or "Sensor Failure" when interacting with the sensors. Users can select a male, female, or cartoon voice by clicking on the appropriate button. Although the imaging application provides default 'sensor ready' and 'sensor failure' WAV files, user can configure their own by selecting the applicable browse buttons to locate and select a different file.
- 'Layout Capture Pause':
  - **When capturing a layout/progression, pause between sensor captures** - This option should be enabled when a sensor system times out too fast or if a certain sensor system needs more time to "reset itself" before it is prepared to capture the next tile in a layout.
  - Enter the amount of time to pause in the text field provided.

- 'Advanced Options':
    - **Display B/C adjustment dialog immediately after single x-ray capture** – Enable this option to allow brightness/contrast adjustments after single x-ray captures.
    - **Ignore "Always Prompt" tiles** – When capturing a layout/series, this option indicates the system should ignore the 'Always prompt for device/sensor' tile option in layout definitions. Images will still be captured for the tile, but the prompt will be overridden.
    - **Activate single x-ray captures immediately** – If enabled, the sensor will automatically be activated during single image captures without the user having to click on the Activate Selected Unit button. This option is useful to users with one or more sensors, from the same manufacturer, that utilize the same hardware drivers.

13.5 Imaging Options and Preferences

Users can access the specific settings of installed extensions for imaging devices such as digital panoramic/cephalometric imaging systems; phosphor plate devices; transparency/ flatbed scanners; and other TWAIN devices. Additionally, user can configure general capture settings that apply to all imaging devices.

- Default Scanner Resolution' - Allows users to set the default resolutions of the images acquired for Periapicals, Bite-Wing Series, Full Mouth Series, Cephalometric, and Panoral. These settings only apply to images captured from a flatbed scanner.
- 'JPEG Image Quality' - JPEG quality factor is an image compression technique that reduces the size of a file to save space on the hard drive. Images can be compressed by as much as 90%, however, the more an image is compressed the more image detail is sacrificed. Apteryx, Inc. recommends leaving the settings to the highest quality feasible.
- 'Layout Stamp Creation' – Select **Create real stamp representations of layouts/progressions** to displays image thumbnails or stamps of the layout as opposed to just gray boxes that represent a layout.
- 'Auto Taken Date Labels':
    - **Automatically place taken date labels** - Option adds a taken date label when a layout is viewed in the imaging application. The label is only applied to images captured after the option is enabled.
    - **Display taken dates in layouts** – If enabled, taken dates will display below each tile in a layout.
- 'Image Acquisition Options':
    - **Twain Devices** - Select this button to access the TWAIN Device Configuration options for any imaging device attached to the system. TWAIN devices require the manufacturer-specific TWAIN drivers to be installed in order for it to be recognized by the imaging application.
    - **Image Device Extensions** - Select this button to access and configure apteryx-supplied extensions for imaging devices such as digital pan/ceph imaging systems and phosphor plate devices. Double-click an available imaging device entry to access the extension settings for post-capture filtration and other device-specific settings.
    - **Select Video Device Type** - By default, the DirectVideo Extension is enabled. Select this button to change to Real-Time Video Extension for older, analog cameras.

13.6 Print Preferences

Users can configure general printing preferences such as page indents; image font sizes; and image size. Additionally, user can configure what patient information to include on the printed image.

- 'Page Indents' - Specify the left/right; top; and bottom page indentations. All measurements are specified in inches.
- 'Fonts' – Users can specify the font type (Arial; New Times Roman; etc.); format (Bold/italicized); and text size is to be applied to Header; Image Information; and Message fonts. To change a font, click on the appropriate font button.
- 'Image Size': - Permit the user to specify how large an image should appear when it is printed directly to a printer.
    - **Full Page** - Indicates that an image should be printed as large as possible on the page.
    - **Real Size** - Indicates that the image should be printed so that measurements may be taken from the printed image. The Real Size setting may crop off a portion of the image if the printed image is larger than the printable are on the printer.

      Due to variances in image capture from imaging devices, measurements in Real Sized images are not guaranteed to be accurate.
    - **% of Page Size** - Indicates the maximum percentage of the page that should be used when printing the image. The image will be appropriately scaled while maintaining the aspect ratio within this percentage of the page.
- 'Printed Image Information' - Indicates what image information (if any) should appear when an image is printed directly to a printer. This information is printed directly below the image.

13.7 Database Preferences

The imaging application allows users to configure database options such as which patient database (local or networked) should be used by the application; what format images should be stored; caching options; and database synchronization options for XV Sync™. Users additionally have access to database utilities and Practice Management data drill options.

XVLite
Preferences
General
Displays options related to the general functionality and operation of the application.
Interface
Displays options related to the interface and general functionality of the application.
Sensor
Displays options related to digital x-ray capture of the application.
Imaging
Displays options related to the various imaging and imaging device handling.
Print
Displays options related to printing images.
Database
Displays options related to the patient database and data formats.
Advanced
Displays advanced options and functions related to the program.
About And Technical Support
Displays technical support and about information for the application.
Language
Enables the user to select the language for the application.
Database Preferences
Database Directory:
This program should use the database in the following directory:
\\Xi3\Users\Stefano\Test2010\Patients
Database contains 3 patient(s)
Database Caching
Use database caching
Database Synchronization
Enable 'To Store' database
Image File Format:
New images should be saved in the following image file format:
STB - Apteryx secure file format
Update Patient Database:
Update Patient Database
Find Images:
Find Images By Date
Data Drills:
DataDrill Options
Data Drill Consulting
Consult Data Drills when opening patients from other applications
Check by patient ID number
Check by patient SS number
Done

- 'Database Directory' - Indicates which local or networked patient database should be used by the application. If this option is not changed by the user, then the software will utilize the local patient database.
- 'Database Caching' - This option requires more memory but can significantly reduce network lag over slow or heavy networks. Enabling the **Use Database caching** option will help reduce delays when looking up patient over Wide Area Networks (WANs).
- 'Database Synchronization' – The **Enable 'To Store' database** option, when enabled, automatically adds all newly acquired images to an index called the 'ToStoreDB'. This feature should only be used in conjunction with XV Sync™, the remote database synchronization application provided by Apteryx, Inc for users with two (2) or more dental office locations. For more information on XV Sync™, contact Apteryx Support at ***877-APTERYX (877-278-3799)***.
- 'Image File Format' - Allows users to configure the file type images should be saved in. If selected the user will be can change the storage format to:
    - **STB** - Apteryx Secure file format – Apteryx's proprietary 16 bit image storage format that guarantees image authenticity.
    - **JPEG** - Standard file format – The space-saving storage format that uses the highest possible quality setting. Image authenticity is sacrificed with this format.
- 'Update Patient Database' - A patient's image database keeps track of the images, tooth information, and image types of the patient. The application automatically checks to see if a patient's image database becomes out of date and will automatically update the database. Should a patient's image database hopelessly become out of synch (i.e. incorrect times and dates on different computers), a user can select **Update Patient Database** to run the utility and rebuild the patient index.

Depending on the size of the database this utility may require a significant amount of time to complete. Apteryx recommends running the utility at the dental facility outside of normal business hours. Contact Apteryx Support at **877-APTERYX (877-278-3799)** for consultation if needed.

- 'Find Images By Date' - Occasionally, users may need to perform a search for an image that was inadvertently captured under the wrong patient. Select **Find Images by Date** to perform a search of the entire patient database for all images captured within a specified date range. Refer to Finding Images By Date (Appendix A) for detailed instructions.
- 'DataDrill Options' - The DataDrill options are used to access the various options associated with practice management bridges. Primarily these options are accessed when changing the database location of a practice management's database. Users can access the Apteryx-provided datadrill, if installed, to change the path to the Practice Management database and configure other options.

13.8 Advanced Preferences

- 'Link to Other Installation' – This option is used to link an application to another networked installation of the imaging application. Linking two installations together allows the programs to use the same layouts, document templates, devices, and definitions; however, the patient databases remain separate. Select **Enable link to …** and then browse to the directory of the other installation on the network to link the two applications together.
- 'Reregister the application' - The **Reregister** button is used when then registration number of the application must be changed. The user should not access this function unless directed to do so by a qualified technician.
- 'Licenses' – Select **Access Licensing** Info to view a list of licensed computers and review the number of available licenses. Licenses can additionally be reallocated or freed up for other computers to use the license.
- 'Auto Saving Images' – When these settings are checked, the program will automatically save a temporary duplicate file on the hard drive. If these settings are not checked and the computer crashes or loses power, unsaved images will be lost.
    - Use non-threaded Safety Cache (TM) applies to older or slower computers such as a 486 or Pentium 100. (Such systems are not recommended.)
    - Use Threaded Safety Cache(TM) – applies to most new computers.
    - Save layouts after each capture - Automatically saves layouts in the patient's file after each tile capture. If this feature is not enabled, the layout must be saved manually after all images are captured.
- 'Slide Show Timer' – This option is used by the software to determine how long of a pause should be performed when displaying the images in a slide show or automatically advancing through the images in a layout.

***** END OF DOCUMENT *****